



System Operation Manual

v 6

Scotia Instrumentation Ltd

Campus 1 Aberdeen Science Park

Bridge of Don

Aberdeen

AB22 8GT

telephone: **UK+1224-222888**

email: support@scotia-instrumentation.com

www.scotia-instrumentation.com

Scotia Data Acquisition System

v6.09

Index

The SDAS System

Introduction	4
Function	4
Overview	5
Starting the SDAS5 unit	6
Shutdown - closing down the SDAS unit	6
Starting the SDAS program	7
Closing down the SDAS program and unit	7
Data Integrity	7
Acquiring Data	7
Graphed Data	8
Reviewing Data	8
Graphics in this Manual	8

Operation of the SDAS program

Starting the SDAS	9
-------------------	---

Menu System

File Menu

Quit	11
------	----

Edit Menu

Edit Menu	11
-----------	----

Data Acquire Menu

Start Acquiring Data	12
Review Stored Data	25
Review Stored Graphs	34
Review Stored Certificates	36
Show Stored Data	37
Delete Stored Data	39
Delete Stored Graphs	41
Delete Stored Certificates	42
Print Stored Data	43

Export/Import Menu

Export Secure Data File	46
Export Data as Text	48
Export Graph File	49
Export Certificate File	51
Import Secure Data File	52
Import Graph File	54
Import Certificate File	55
Export Equip File	56
Export User File	57
Export Levels File	57

Export Certs Labels File	57
Export Setup Labels File	57
Import Equip File	58
Import User File	59
Import Level File	59
Import Certs Labels File	60
Import Setup Labels File	60

Test Equipment Menu

List Equipment	61
Create Equipment	62
Amend Equipment	64
Cal of A to D	65
Get Connected Chip IDs	71
Get Connected Transmitters	71

User Menu

List Users	72
Create User	73
Modify Users	74
Modify Level Access	75
Change Current User	77

Utilities Menu

Print Setup	78
Restart Setup	78
Set Comms Port	79
Toggle Setup Pallet	80
Toggle Print to PDF	81
Toggle Auto File Save	82
Toggle Calibration Date Check	83
View System Log	84
Set Logo	86
Refresh the Data Lists	87
Restore Menu Bar	87
Which System	88
File Browser	88

Settings Menu

Set Company Name	90
Set Customer Name	90
Set Default Interval	91
Set No of Channels	91
Set Channel Labels to Default	92
Set Default Load/Save Locations	93
Set System Save Location	94
Set Certificate Labels	95
Set Certificate Type	95
Set Data Pallet Labels	96
Set Next Data Label	97
Set Graph Limit	98
Set Data Listing Limit	99

Other SDAS Devices

Starting the SDAS program on a PC	100
ScotiaLogger3	101
SUDS	104

SDAS Options

Counter Options	107
Variable Data Rate Option	111
Hold Period Timer Option	111
Test Event Log Option	113
Alarm Option	115
Certificates Option	118
Door Alarm Option	127
Test Event Marking Option	128
Enhanced Data Entry Option	131
Recalibration Due Option	141
Export Test Data at Finish	142
File Browser	143

SDAS5 Hardware

SDAS Unit front	145
SDAS Unit back	145
SDAS5 Specification	148
Scotiadatabox Unit	149
Spares and Accessories List	150

Appendix 1

Starting the SDAS unit	151
Shutdown - Shutting down the SDAS unit	151
SDAS - Launching the SDAS program	153
Help - Operation manual pdf	153
Printers - Changing printers	154
Files - Access local files	154
Switch User - Change User	155
Technician Menus	155
Technician Network button	158
Technician Support button	159

Appendix 2

4D Error Messages	160
-------------------	-----

The SDAS System

Introduction

The Scotia Data Acquisition System (SDAS) is available in several versions which operate with the SDAS family of products. The main SDAS devices are the SDAS4 and SDAS5 which have 8 channels. If fewer channels are used then these disable automatically avoiding any operator confusion with dead channels. The transmitters used have chipped plugs which interact with the program to load all range information automatically.

A PC or PC laptop can be used with a Scotiadatabox to gather the data in real time in a manner identical to the SDAS. The database program for the SDAS also operates on a PC or PC laptop to upload data from the Scotialogger3, Scotialogger4 and Scotia Underwater Datalogger System (SUDS) devices which are all standalone loggers with visual indication. The SUDS is a remote device which can operate as a standalone device in depths of up to 3000m. All of these devices download their data into the SDAS program running on a PC allowing all the functionality and data analysis of the main SDAS together with the security of the data link ensuring that data cannot be altered by the user in any way.

The current version of the SDAS program is version 6 and all screen captures shown in these instructions are from SDAS-6 program running on the SDAS5 device. Variations for other members of the SDAS family are shown in the Appendices.

The SDAS5 can have up to eight 4-20mA inputs, two Pt-100 inputs, and up to three counter inputs. Rising or falling alarms can be set for each of the 4-20mA inputs.

The hardware of these units have been extended with additional functions which have been developed to meet the needs of certain customers but these instructions deal with the basic SDAS unit. Additional functions of the other hardware units and options available on the SDAS are covered in the Options section. The Review version of the SDAS-6 program, which is used to view and process data gathered by an SDAS and exported to a PC is also covered in this section.

Function

The SDAS will gather data from 4-20mA analogue transmitters, Pt-100 temperature probes, and pulsed counters. The 4-20mA signal can be from a pressure transmitter but this can be any 4-20mA signal giving any value of units. Where 'pressure measuring' is used in the following text any measurable quantity could be substituted. The data is digitised and stored within a database together with date, time and data labels making a packet of data which can be retrieved at any future time in part or as a whole test. The data can then be viewed, exported to disk, or displayed graphically on screen or printed either graphically or as numerical data.

While gathering the data from the input devices, the program shows the data on screen both graphically and numerically. The system runs two program loops simultaneously while operating. The main primary loop gathers data from the analogue to digital part of the system and logs these values to disk. The secondary loop takes this data and displays it in real time. The secondary loop can also be used to review gathered data while the primary loop continues to gather new data. This allows the technician or inspector to examine gathered data and even print this data graphically while the primary loop continues to collect data.

Access to data can be restricted by a sophisticated password access system allowing a system administrator to control access down to the level of screen buttons.

Data cannot be altered in the database in any way other than deleting it. This gives a secure record system which gives an absolute assurance that data recalled can have been neither tampered with while being gathered nor altered in any way since.

Overview

The structure script controls the input to a database using a 4th Dimension database engine. The database filing system makes searching for stored data and recalling it a simple and reliable matter given reasonable care initially with labeling etc. Data is logged to disk within the SDAS unit and any power failure or other acquiring interruption will only affect the data event currently being gathered. Previously gathered data will be safely stored to disk.

The data is shown graphically and numerically during the acquiring process and the event window can be re-scaled as you require. Pressure and temperature are logged on separate graphs within the graphing screen using the same time scale. The SDAS receives the 4-20 mA signal and ranges it to match the range of the transmitter. Each transmitter and temperature probe must be registered in the system and, if the transmitter has a serial number chip fitted, it and the range are entered automatically by the system when it is used. The range can be reset by the user by numerical conversion from the transmitters calibrated range.

The time and date of the events are noted at the time of acquiring on the computer used. The graph time scale is shown as events marked by their received time.


Minimum screen depth for use is 1024 x 768 and the screen will dynamically enlarge the graphing areas as the screen size available for use increases.

The program has an on-screen help function. This brings up an info box about controls and data fields as the mouse pointer is moved over them. The box appears after a few seconds and disappears again after a few seconds. The info field appearing does not affect the operation of the buttons or fields.

Starting the SDAS5 unit

The SDAS units are started by switching on the physical power button. The SDAS has a basic interface screen along the bottom of which is a task bar from which you can do various tasks. These include shutting down the SDAS safely, starting the main SDAS application, viewing the SDAS manual, access file functions, access printer operations, access advanced configuration, noting the operating system version, registration status and setting the current time. The following screen appears when the system starts up.

The button bar will disappear when the SDAS program is launched or you place the mouse close on it. Placing the mouse near the bottom of the screen will make it reappear.

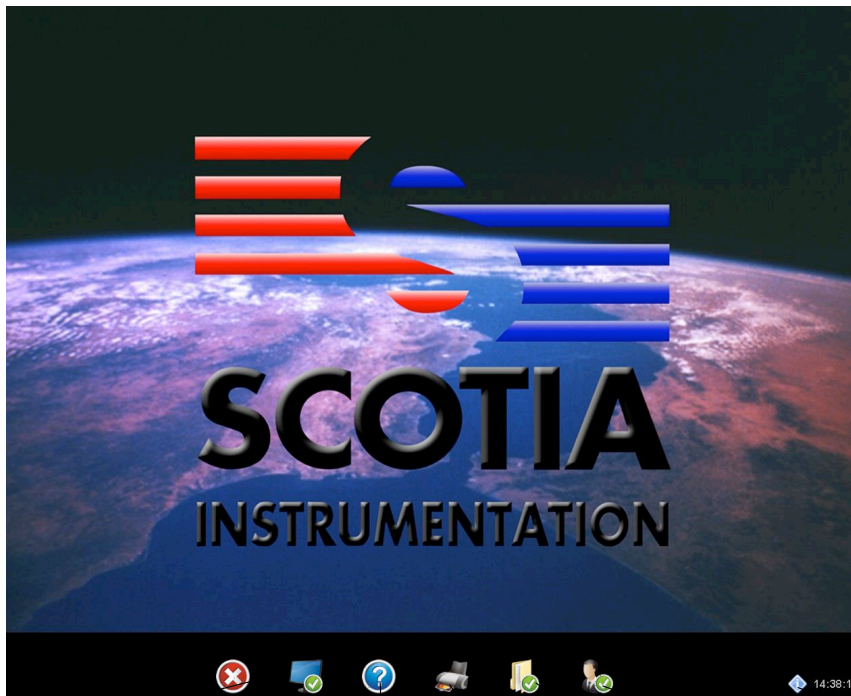

Note that the button bar will disappear when the SDAS program is launched. Placing the mouse near the bottom of the screen will make it reappear.



- Safely shutdown the SDAS
- Launch the SDAS application
- View the SDAS Manual and Help
- View Printer configuration panel
- Access File browser
- Switch user to access Configuration menus
- Software build version information
- Current Time

When you first start the SDAS the above panel will appear. The Control bar along the bottom will stay in place until you launch a program or hover your mouse on it. After that the bar will hide out of sight until you move your mouse close to the bottom of the screen, when it will reappear after a slight delay.

Shutdown - Closing down the SDAS unit

The shutdown button safely shuts down the SDAS unit. When pressed you will receive a confirmation dialog or if the SDAS application is still running you will be prompted to shut down the SDAS application first. Once you have closed the SDAS application you will need to click the shutdown button again.

normal shutdown confirmation

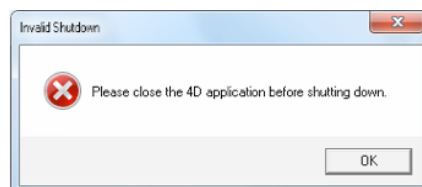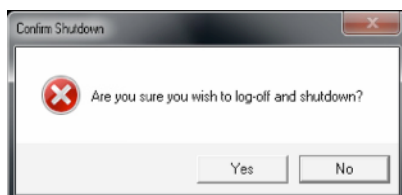

Incorrect shutdown close the SDAS application from the file menu.

SDAS - Launch the SDAS program

The SDAS button will launch the SDAS application.

The other functions of this screen are covered in Appendix 1 of this manual

Starting the SDAS program

Once launched the group login screen appears. The group user name will be '-User1' or '-User2' and the password is 'U' in both cases. Note that this is in uppercase. Each user can only be a member of one group so choosing the wrong group will result in the users name not appearing on the list for choosing on the next screen. The user chooses his or her name from the pop-up list and enters their personal password. The Scotia Data Acquisition System splash screen then appears.

Closing down the SDAS program and unit

The SDAS-6 program should be exited by choosing quit from the file menu. This closes the system functions saving all buffered data as it does so. Once the SDAS-6 program has quit the operating system should be closed down by choosing Shutdown from the screen tab. Loss of buffered data may result if this sequence is ignored.

Data Integrity

The data being acquired by the program to the data file cannot be altered by the user in any way. Received and logged data is kept exactly as produced from the SDAS at the time the data was gathered.

Acquiring Data

Acquiring is done to the data file at the time interval set. This file is held within the SDAS program's data file and is stored on the SDAS's hard disk and all data received by the SDAS will be buffered and saved to this disk file as it arrives, no matter what the graph indication is being asked to do. If the SDAS fails, for any reason, then all the data up to that point will have been saved to disk automatically other than possibly what is held in the 60 second memory buffer.

When acquisition is stopped, it can be restarted either to the same data file label or as a new data file label. If you restart with the same label then the time axis will not 'look' linear. The events on the graphs will be labelled with the correct receiving time but any period that the acquisition is stopped will not be reflected with a gap in the graphing time line. All events like start, stop and pause will be noted in the test log.

Note that the SDAS-6 structure is running concurrent routines. This is not true multitasking. The computer running any other part of the program may miss acquiring if another routine is sufficiently 'distracting'. User input will capture a lot of the computer's attention. For example, holding a scroll button continuously or waiting while deciding on print settings if you are viewing data in Review may be enough to cause a data capture to be missed. If this happens the program will always advise you as soon as data has been missed but this may be small consolation when you have to stop logging and restart and miss a logging point.

Each data item received in the Scotia Data Acquisition System has saved with it;

The data label entered at data start containing the Test ID number, Serial number of the SDAS unit, the operating technician's initials and any additional label data.

The User ID label entered

The serial numbers of the transmitters and temperature probes used

The transmitter and temperatures values together with the units of these.

Any offset applied to the transmitter reading at the start of logging.

The program adds the actual computer time and date at which the data was received by the SDAS.

The received events are numbered in the file in the order they are received.

If no temperature probe is being connected to the SDAS then the temperature is noted as -999. This is unlikely to be mistaken for a real temperature.

If zero mA is received on any 'on' channel then this is interpreted as -25% of the scale set as 4mA is considered zero.

Graphed Data

The time axis of the displayed graphs are simply labelled with the arrival time of the data. The time line is not necessarily linear and any delay caused by interruptions or pauses will not appear as gaps in the time line. They will always be labelled correctly though.

A limit of 250 graphed events is set for the gathering data graph. After this the graph scrolls left out of the time scale.

Reviewing Data

The Review mode offers an analysis package for the data currently stored within the SDAS database. The data review can operate either while acquisition is operational or not and on data currently being acquired or on stored data with a different data label.

The graphing process uses a memory array system to store the data for the graphs. If you are operating with large amounts of data then even the fastest computers will give slow performance and older PCs may crash if the processing gets too much for it. In order to restrict the demand for large amounts of operating RAM data events numbering in excess of 10,000 items will either be divided into 10,000 item parts for Review graphing or sampled to reduce the data to within 10,000 items. This process does not change the stored data in any way.

Graphics in this Manual

The screen captures used in the main part of this manual are taken from the SDAS at version 6 running on an embedded version of Windows 7. The SDAS program is continually evolving so screen graphics in later versions may vary slightly from this.

The screens shown may have additional parts which appear only when options are added to the basic unit. The options section will illustrate these differences.

The access level system allows user access to various parts of the SDAS routines. If your access is restricted you may be unable to use certain routines. You will be advised of this when you try to access these areas.

Print to PDF

From version 6.07 printing to pdf is a standard option. The pdfs created are saved to the default save folder or, if the path to it has been lost, to the internal system save folder.

Starting the SDAS


Connect all components to the SDAS before starting the SDAS device. The SDAS system should be started by physically switching on the power to the unit. This starts the AtoD system and the main SDAS-6 operating system. Once loaded the system start screen shows like this.



Launch the SDAS application by clicking this icon

Launch the SDAS system by clicking the SDAS icon. The SDAS program then starts and the Group Access password screen appears.

Group Access Password Screen

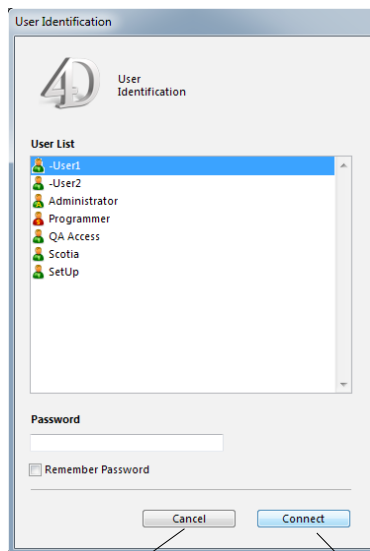

Choose the User Group access name and enter the User Group password

The default access code for both groups -User1 and -User2 is 'U' (capital u)

Cancel quits from the SDAS system

Confirm to proceed to user name and password entry


If an incorrect access code is provided then the system will not proceed. Cancel is your only exit.

Successfully entering a Group Access Name and its password then leads to the individual password entry screen. Only users in the Group just entered will be offered as a choice for user name entry.



The user chooses their name from the pop up list and then enters their password. The default user is Test Person with a password 'TP1'. The user proceeds by clicking Confirm. If the user does not see their name or cannot enter a valid password then they only have the option to Quit System. The SDAS splash screen appears after successful logging on and the rest of the system is accessed by the menus which follow.

This shows the current SDAS version This shows the options active in this SDAS version. This shows the serial number of the SDAS in use. This shows the name of logged in current user.

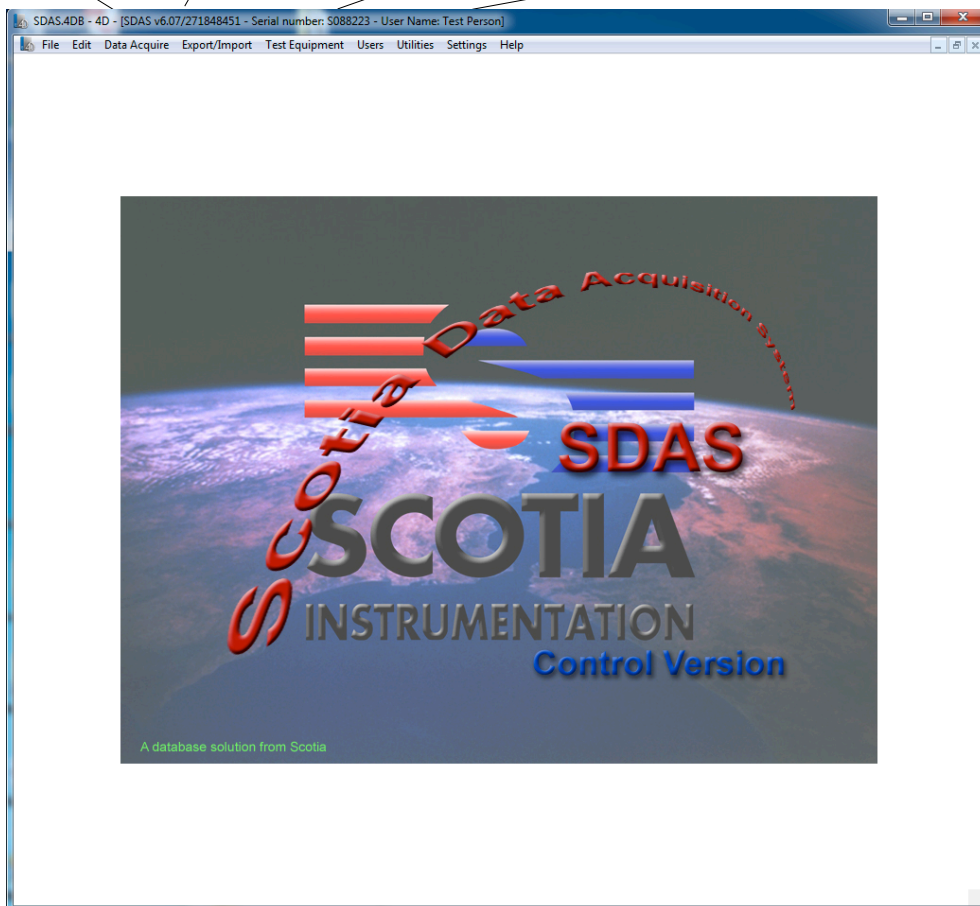


This is the main screen of the SDAS-6 program. All functions are started from the menus at the top of this screen. The menu functions will be covered in the following instructions.

Menu System

The SDAS system is driven from a menu system of the main splash screen. Each menu is shown and explained in order of their appearance on the screen.


File Menu

Quit



This exits the SDAS-6 program and returns to the SDAS system start screen. Exiting this way ensures that the system closes all open files and saves down all data buffered in memory.

Edit Menu


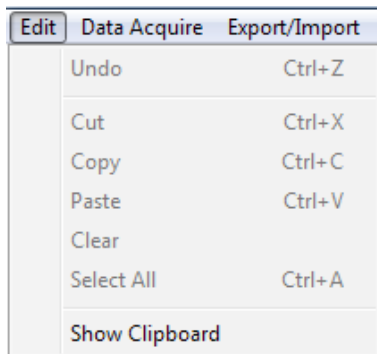


This menu performs system functions and is not selected by the user directly

Data Acquire Menu

Start Acquiring Data

This is the routine that acquires data into the SDAS. The transmitters and temperature probes should be connected to the SDAS unit before starting the SDAS unit.

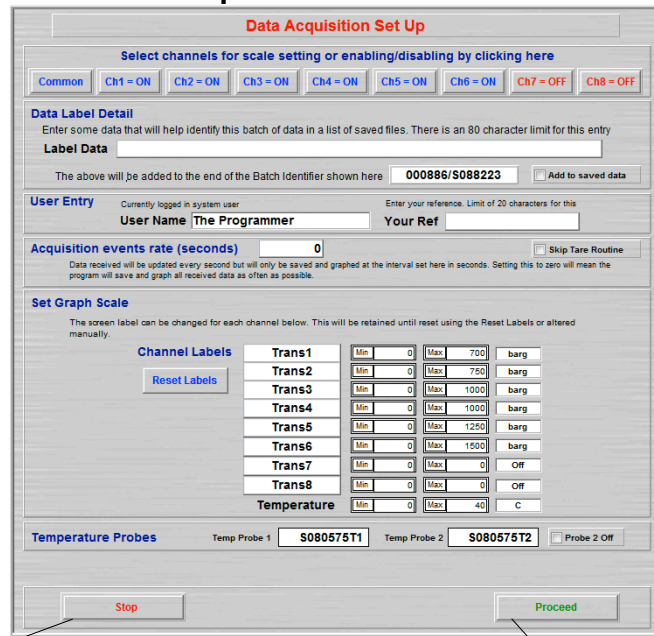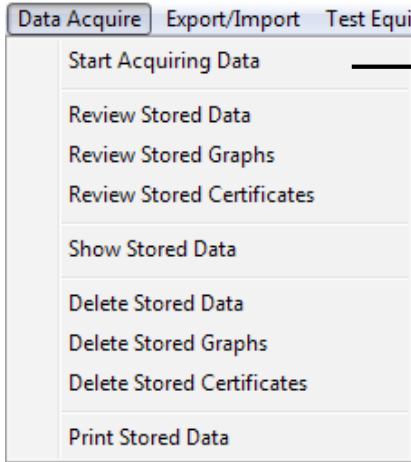


If chipped transmitters are used then those channels load automatically. If not then an alert is shown and the channels are switched off and are switched on when selected and you must choose the connected transmitter from the pop-up serial number list. Range and units are added from the data held in the system. Channels with no transmitters connected cannot be left on.

This stops this routine and returns to the main screen.

This leads to the next screen

The operation of this screen has several components and to aid explanation the screen will be divided into these parts



Clicking on any of the active Ch buttons takes you to the setup screen for that channel. Any channel that does not have a chipped transmitter will appear set to Off here. It can be turned on by clicking on it and selecting a transmitter from the pop up list of serial numbers.

The range set for each channel in these screens determines the range for any graph showing that channel. The scale is set to the largest range of the channels currently showing on the graphing screen.

This shows the screen for setting channel 1

If a chipped transmitter is used then the serial number is loaded here automatically and this field is disabled. If not then you must choose a transmitter from the pop-up list to proceed

The range is entered automatically and cannot be altered by the user here. The range is entered from the data held by the system for that transmitter. The transmitter range and/or units can be changed in the equipment section of the program.

The graphing scale can be set here

This stops the Setup routine and returns to the main menu screen

This toggles this channel on or off. Any channels set off here is then for the duration of this data session and will not appear on any chart or data file

This returns to the opening Setup screen

When opened this entry is blank - an example entry has been added for illustration. The user can enter an additional data label up to a limit of 80 characters.

This forms the first part of the data label. The first part is unique to this data file and is supplied from the file as the next available. The next part is the serial number of the SDAS being used. These cannot be altered by the user.

This test can be added to the end of another test by clicking this. You will then be asked to choose the data file to use. This has been added to allow a test to be continued after an interruption. Be sure you know what you are doing with this option as you may end up with some strange data files

The current user name is given here and cannot be altered in this screen. The current user can be changed either by restarting the SDAS or from the Utilities menu or during a test from the Change User button.

A user reference can be entered here. This is restricted to 20 characters but otherwise can be any combination of alphanumerics. An existing reference can be entered. Using the same reference can be used to group tests together for review. A search will find them all and list them

Acquisition events rate (seconds) Skip Tare Routine

Data received will be updated every second but will only be saved and graphed at the interval set here in seconds. Setting this to zero will mean the program will save and graph all received data as often as possible.

This sets the rate in seconds that data is gathered into the database file. The digital display is updated every second but the graph and data file are updated at the rate set. The initial setting is to the default value which can be altered in the Utilities menu. Setting the rate at zero will gather data as often as possible. Currently this is 1 per second.

If checked then this skips the Tare routine. This avoids the pause to check the zero setting of the transmitters

Set Graph Scale

The screen label can be changed for each channel below. This will be retained until reset using the Reset Labels or altered manually.

Channel Labels

Trans1	Min	0	Max	700	barg
Trans2	Min	0	Max	750	barg
Trans3	Min	0	Max	1000	barg
Trans4	Min	0	Max	1000	barg
Trans5	Min	0	Max	1250	barg
Trans6	Min	0	Max	1500	barg
Trans7	Min	0	Max	0	Off
Trans8	Min	0	Max	0	Off
Temperature	Min	0	Max	40	C

The default labels of the transmitters can be changed here to a more meaningful label for a user's test. This labeling is used on the screens and printed test results and are saved with the data

The scales of the 4-20mA channels are set on their channel screens as described above and are disabled here

The temperature graphing scale can be set here

Labeling Channels

Set Graph Scale

The screen label can be changed for each channel below. This will be retained until reset using the Reset Labels or altered manually.

Channel Labels

LineA	Min	0	Max	700	barg
LineB	Min	0	Max	750	barg
MidLine1	Min	0	Max	1000	barg
MidLine2	Min	0	Max	1000	barg
Main1	Min	0	Max	1250	barg
Main2	Min	0	Max	1500	barg
Trans7	Min	0	Max	0	Off
Trans8	Min	0	Max	0	Off
Temperature	Min	0	Max	40	C

Temperature Probes Temp Probe 1 Temp Probe 2 Probe 2 Off

The labels can be reset to the default by clicking here

Some sample labeling is added here

The labeling is retained for further tests until the Reset Labels is clicked or the label is changed here

This is the serial number of the temperature probes connected to Temp 1 and 2 input. This must be entered in the Equipment file. If not then you are advised of this and cannot proceed until you have entered it.

Note that the temperature probes graph on the same scale. If a probe is not connected then the system will give an output of -999 degC for that probe as zero would be misleading. A constant -999 will distort the shared graph in Review mode or when Auto is checked. To avoid that you can check the Probe 2 off box. Probe 2 will then be ignored and not graphed.

When Proceed is selected in the above screen the connected transmitters are read by the system over 5 seconds and an average of those values is shown in the Zero Offset screen below. This allows any zero offset of the transmitter to be removed if required before any test starts. Any offset chosen here will be logged with the data. This allows any amount zeroed in error to be explained or corrected later.

Zero Offset

Zero Offset Transmitters

Data Label: 000886/S088223/ZTP/TS001

LineA	S080558ch1	Range	0	to	700	barg
LineB	S080558ch2	Range	0	to	750	barg
MidLine1	S080558ch3	Range	0	to	1000	barg
MidLine2	S080558ch4	Range	0	to	1000	barg
Main1	S080558ch5	Range	0	to	1250	barg
Main2	S080558ch6	Range	0	to	1500	barg
Trans7		Range	0	to	0	Off
Trans8		Range	0	to	0	Off

Transmitter 1 Currently Reads	-0.14	Offset this to the 0 barg value	<input checked="" type="checkbox"/> Set
Transmitter 2 Currently Reads	-0.0375	Offset this to the 0 barg value	<input checked="" type="checkbox"/> Set
Transmitter 3 Currently Reads	0.49333	Offset this to the 0 barg value	<input checked="" type="checkbox"/> Set
Transmitter 4 Currently Reads	1.06	Offset this to the 0 barg value	<input checked="" type="checkbox"/> Set
Transmitter 5 Currently Reads	0.70417	Offset this to the 0 barg value	<input checked="" type="checkbox"/> Set
Transmitter 6 Currently Reads	0.575	Offset this to the 0 barg value	<input checked="" type="checkbox"/> Set
Transmitter 7 Currently Reads	0	Offset this to the 0 Off value	<input checked="" type="checkbox"/> Set
Transmitter 8 Currently Reads	0	Offset this to the 0 Off value	<input checked="" type="checkbox"/> Set

Transmitter values shown in red exceed the recommended amount for offsetting. Those in green may have non-zero values.

The transmitter labels, serial numbers and range are displayed here.

The output from the transmitters are sampled for 5 readings and the averages are shown here. If the value is more than 5% of the span then this value shown in red. If the bottom range value of the transmitter is not a zero amount then this is shown in green. Red or green coloured values are deselected automatically for offsetting and you must be clear you know why if you do offset these.


If the reading from the transmitter is below 5% and the lower range value is zero then this is checked automatically. It can be checked manually. When checked the current reading will be offset from any values read from the transmitter. The operator is expected to know when this is a normal zero offset and when a 'real' value is currently on the transmitter. 'Real' values should not be reset to zero as this will give a false reading from the transmitter for this test. The data for each point will have this value correction noted.

This continues to the next screen without applying any suggested offset.

This applies the suggested offset if Set checked and leads to the next screen

Acquisition Display

Before acquisition of data starts this screen loads with blank graph areas and transmitter value displays show Ready as no value has been read from any transmitters or temperature probes yet

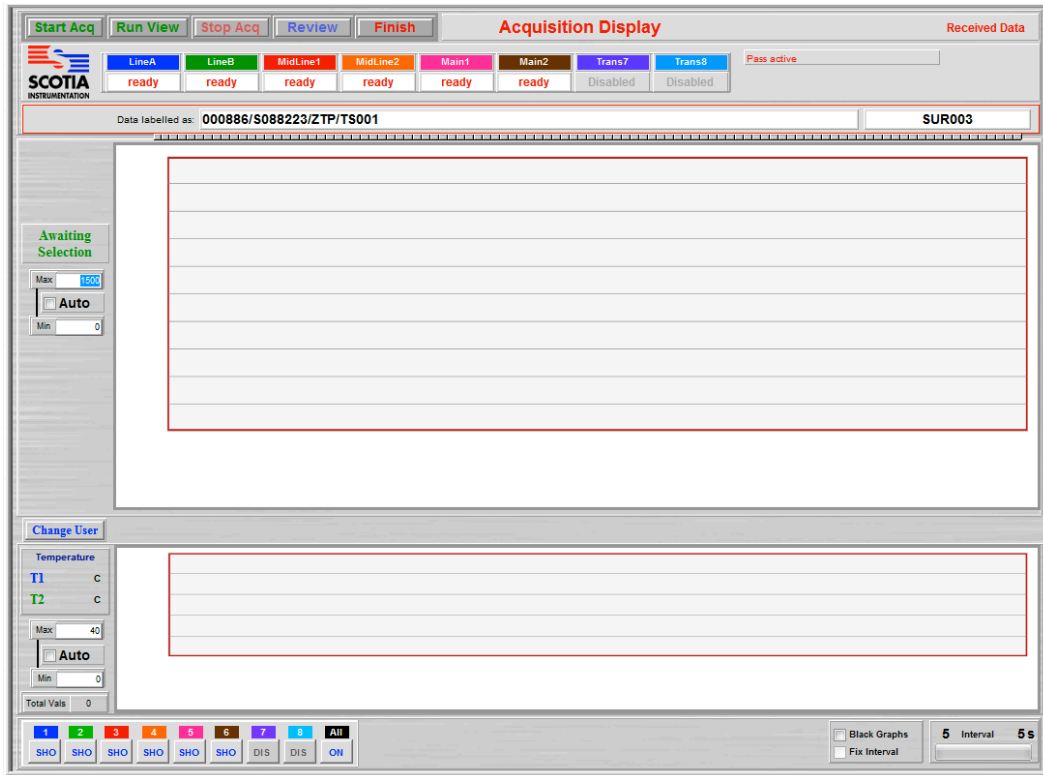

The operation of the Acquisition Data Display screen has several components and to aid explanation the screen will be divided into parts

Control buttons


Acquisition can be started, stopped and restarted with this button

Once acquisition has started this becomes active and leads to the Review mode

This finishes any running routine, closes this screen and returns to the main screen



This runs the acquisition routine showing the current readings but does not save or graph the data.

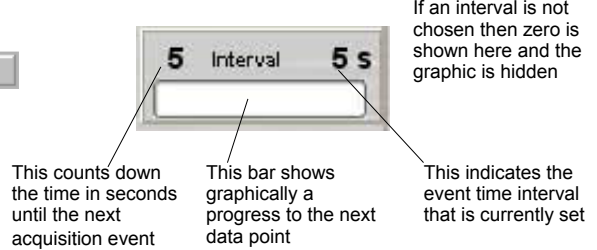

This counts down the time in seconds until the next acquisition event

This bar shows graphically a progress to the next data point

If an interval is not chosen then zero is shown here and the graphic is hidden

This indicates the event time interval that is currently set




This shows the current data label for acquisition

The data label comprises of the following components;


- 000806 - This is the unique system ID.
- S088223 - This is the unique SDAS serial number and identifies the SDAS unit being used. This should be the same as the Serial Number on the back of the SDAS unit.
- TP1 - This is the identifier of the current user.
- TS001 - This is the text identifier added by the user and can comprise of any text. The limit for this part of the label is 80 characters.

This shows the user reference

Transmitter Readings

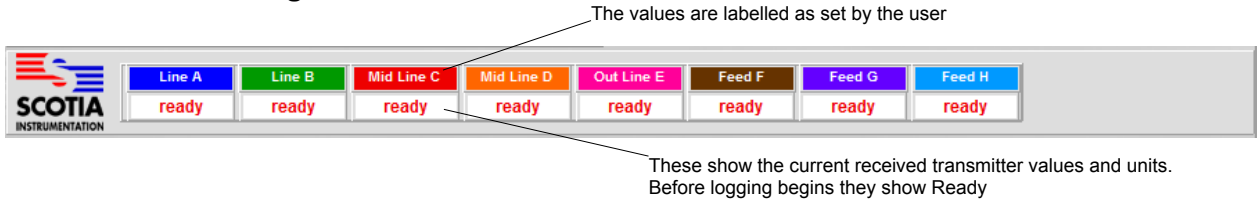

Value Axis Ranging

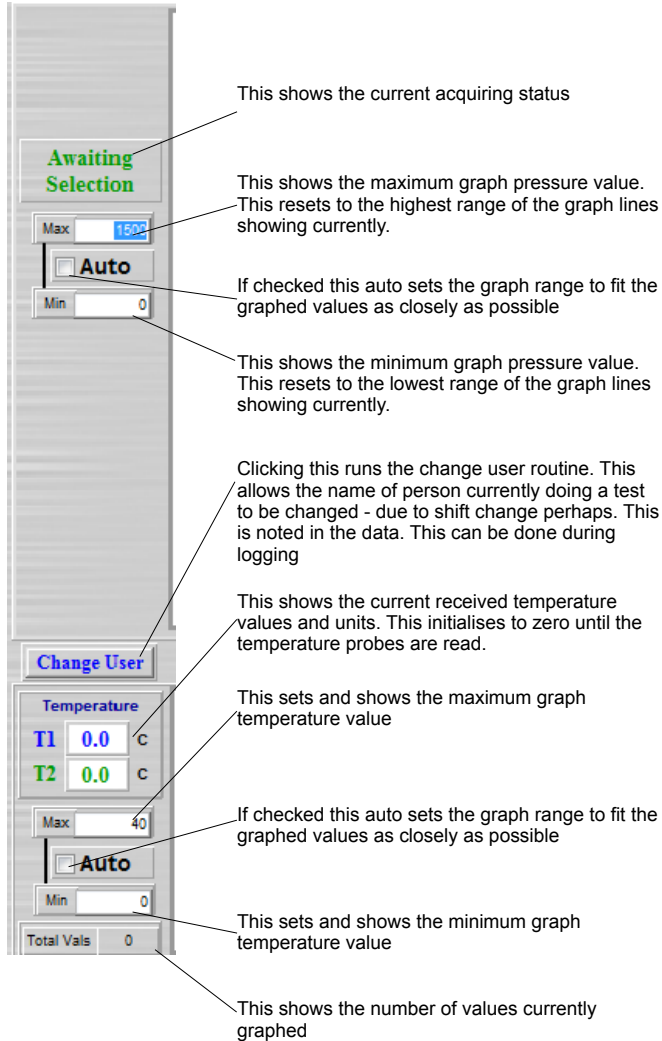


Channel Selection



These control the channels displayed - clicking a channel control toggles it from on SHO to off HID. Any channel not selectable is shown as disabled DIS. 'All' allows all channels to be selected as on SHO. The colours on the channel labels match the colour of the graph line. Note that you cannot show no channels. If only one channel is showing and you click on it to switch it off then nothing will change. The toggle action operates to this rule: if All is ON then clicking any channel switches to just show that channel. If all the channels have been switched on by clicking on them then clicking on any one simply switches that channel off and leaves the others on. The display of the channels on the graph only changes at the next logging event when the graph updates.

Graph appearance

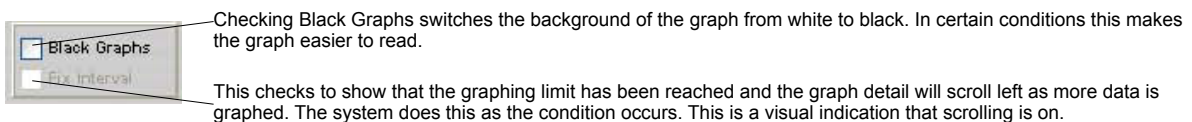


Graphs

These are the pressure and temperature scales

Clicking on this bar will remove the graph up to the left of the point clicked. Only the display is affected by this action

This shows the graphed transmitter values

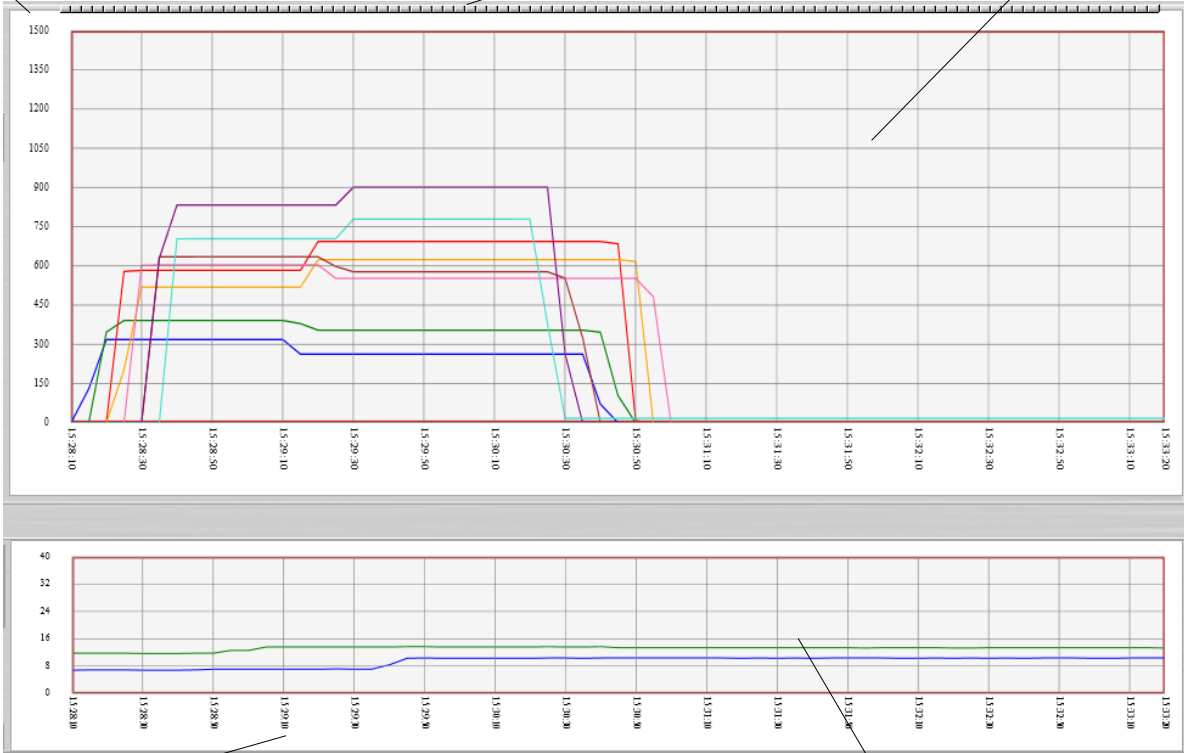

This is the time label showing the time the data item was received by the SDAS. The two graphs have the same time scale.

This shows the graphed temperature values

If the transmitters are not all in the same measurement units then a graph showing mixed units will show in percentage 0-100 and each scale is shown as a percentage of its range. When the channels selected for showing are all the same units the scale switches automatically to show the range of the greatest channel in the scale of the shared units.


This shows an example screen receiving data

When receiving data these buttons alter to this form. Note that Start Acq has changed to Indicate that the routine is running. Run View is no longer selectable. Stop Acq is now active as is Review and Finish.

Review does not activate until eight data events have been stored. The button label indicates the countdown and is inactive. If the user access level does not allow reviewing while logging then this button will always be disabled here

These show the current received values on the transmitter channels. These are updated every second regardless of the logging interval

This shows the current time and date being stored for acquired data.

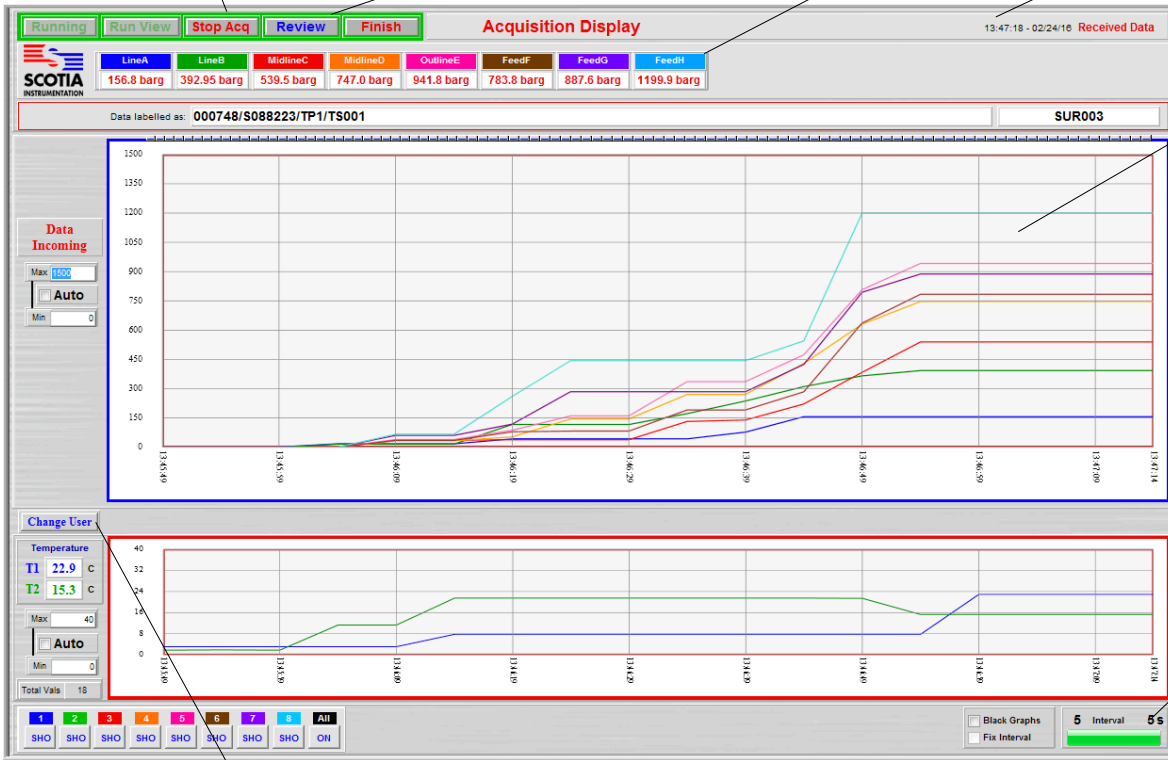

The graph areas are dynamic and will size according to the available screen area. The surrounding graphics remain the same size.

This shows the seconds until the next data logging event with the graphic.

The Change User button allows the current user of the system to be changed. The system logs who is the current user and any change. This allows the current user to be tracked where tests may be running over the shift of more than one test person.

When Stop Acq is clicked these buttons change to the following. Note that Running has changed to Restart. Run View is now selectable. Stop Acq has now changed to Stopped and is inactive.




If enabled clicking Review leads to the following screen

Review Acquired Data

Clicking the Review button while either still acquiring or with acquiring stopped will lead to this screen.

Reviewing while logging can be prevented in the Levels section of the system. If the user has a Level access which prevents that the Review button is not active.

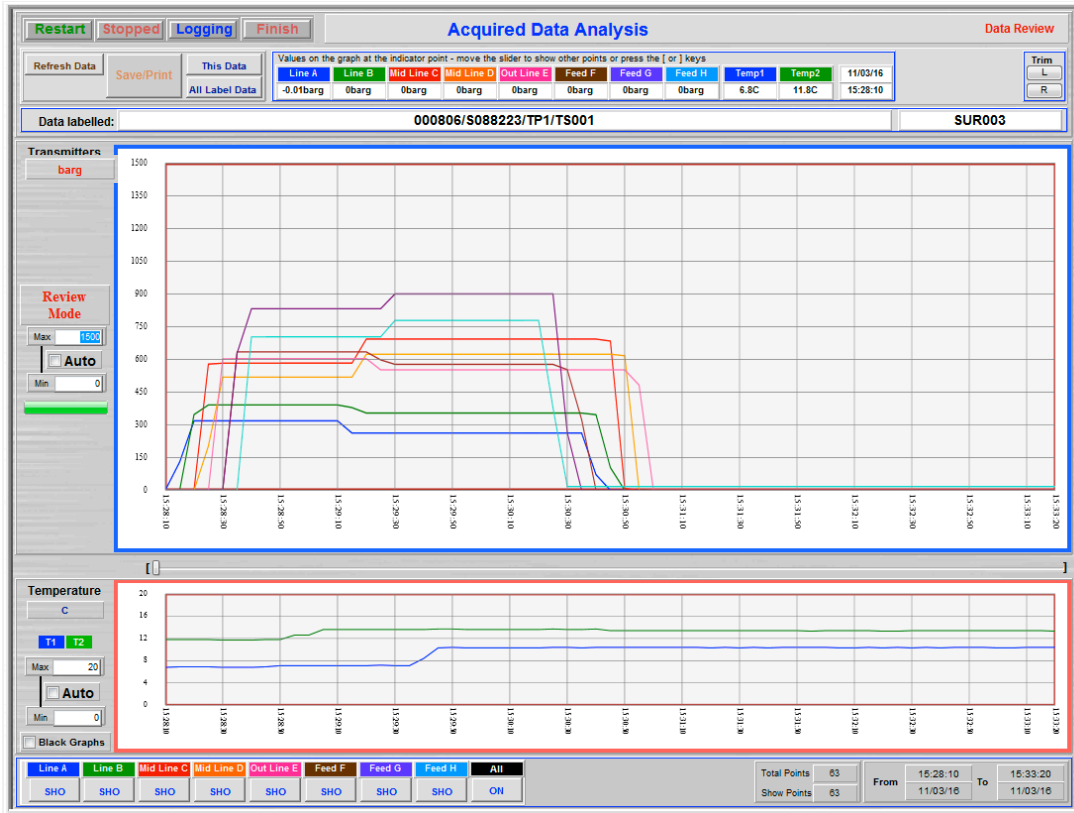

The graphed data shown here does not update with new data when the data is still being acquired. The Refresh Data button needs to be used to manually update to the latest data.

The operation of the Acquisition Data Analysis screen has several components and to aid explanation the screen will be divided into parts

This restarts acquiring if it has been stopped

This is a visual indicator of logging - Stopped indicates logging stopped

This returns to the acquiring screen

Values shown here when the screen opens are for the left side of the graphs

L-R trimming - Used in conjunction with the Location marker - clicking L or R will move the left or right end of the graph up to the Location Marker.

This shows the Transmitter units. If more than one unit is being graphed then this shows 'various' and the graph shown is in percentage

Clicking here gives a pop up list of the saved data files labels. Selecting from the list will load that file into the Review graphs below even if acquiring is continuing to the original file.

Clicking here gives a pop up list of the saved User labels. Selecting from the list will load that file into the Review graphs below even if acquiring is continuing to the original file.

Reviewing other data while logging can be set in the Levels section of the system. If the user has a Level access which prevents that these items are not active.

This resets the graph to show all the current label data stored

This is the current mode identifier


While Auto is checked the graph will autorange in the values axis to best fit all currently shown graphed values. If unchecked the graph range is set by typing values into the Max and Min boxes. Note that moving the cursor out of the range box activates the change.

This is a visual percentage indicator of the amount of data showing for the current data label.

This shows the colour coding of the graphed temperatures

While Auto is checked the graph will autorange in the values axis to best fit all currently shown graphed values. If unchecked the graph range is set by typing values into the Max and Min boxes.

If checked this sets the graph to display on a black background

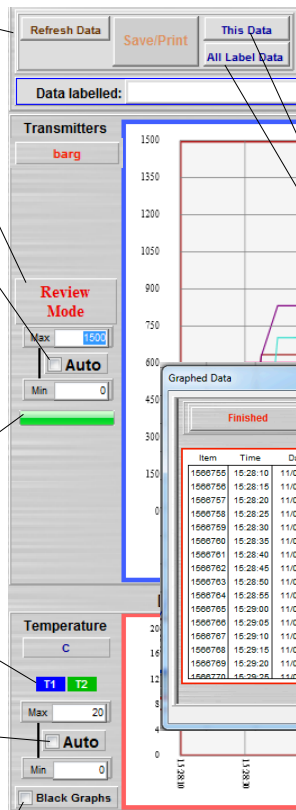

Clicking the This Data or All Label Data gives a floating display of the current data label values. 'This Data' shows the data currently graphed and 'All Label Data' shows all the data saved for this label. The list can be scrolled and the floating display can be moved around the screen if required. The graph loads with the start and finish values being either the range of the currently showing graph or all the label data. It can be used to set the Graphs to a new range of values by clicking on the required start value and then clicking on the required finish value on the listed values. The from and to values update as you do so. You can reselect by repeating this action. Clicking Regraph will select this range for graphing. Clicking Finished will just restore the current graphing range.

Graphed Data

Finished Regraph

Stored Data Values


Click on the listing to select the start and finish points

Item	Time	Date	Trans 1	Trans 2	Trans 3	Trans 4	Trans 5	Trans 6	Trans 7	Trans 8	Counter 1	Counter 2	Counter 3	Temp 1	Temp 2
1566755	15:28:10	11/03/16	-0.01	0	0	0	0	0	0	0	-1	-1	-1	6.80	11.80
1566756	15:28:15	11/03/16	129.68	0	0	0	0	0	0	0	-1	-1	-1	6.90	11.80
1566757	15:28:20	11/03/16	318.19	347.12	1.1	0	0	0	0	0	-1	-1	-1	6.90	11.80
1566758	15:28:25	11/03/16	318.19	391.19	576.7	203.1	0	0	0	0	-1	-1	-1	6.90	11.80
1566759	15:28:30	11/03/16	318.19	391.2	583	518.7	602.6	2.2	0	0	-1	-1	-1	6.80	11.70
1566760	15:28:35	11/03/16	318.2	391.2	583.1	518.7	603.7	634.6	629.3	0	-1	-1	-1	6.80	11.70
1566761	15:28:40	11/03/16	318.19	391.21	583	518.7	603.7	634.6	632.5	703.5	-1	-1	-1	6.80	11.70
1566762	15:28:45	11/03/16	318.19	391.21	583	518.7	603.7	634.7	632.5	703.8	-1	-1	-1	6.90	11.80
1566763	15:28:50	11/03/16	318.19	391.21	583.1	518.7	603.8	634.7	632.5	703.8	-1	-1	-1	7.10	11.80
1566764	15:28:55	11/03/16	318.2	391.2	583.1	518.7	603.7	634.7	632.5	703.8	-1	-1	-1	7.10	12.00
1566765	15:29:00	11/03/16	318.2	391.23	583.1	518.7	603.7	634.7	632.5	703.8	-1	-1	-1	7.10	12.00
1566766	15:29:05	11/03/16	318.2	391.21	583.1	518.7	603.7	634.7	632.5	703.8	-1	-1	-1	7.10	13.00
1566767	15:29:10	11/03/16	318.19	391.23	583.1	518.7	603.8	634.7	632.6	703.8	-1	-1	-1	7.10	13.00
1566768	15:29:15	11/03/16	262.3	379.28	583.1	518.7	603.7	634.7	632.5	703.8	-1	-1	-1	7.10	13.00
1566769	15:29:20	11/03/16	262.3	354.08	593.4	623.9	603.8	634.7	632.5	703.8	-1	-1	-1	7.10	13.00
1566770	15:29:25	11/03/16	262.3	354.07	593.4	623.9	603.8	634.7	632.5	703.8	-1	-1	-1	7.20	13.00

from 1566755 to 1566817



These control the channels displayed - clicking a channel control toggles it from showing SHO to hidden HID. Any channel not selectable is shown as disabled DIS and does not show on the graph. All allows all channels to be selected as showing SHO unless they are currently DIS. The colours on the channel labels match the colour of the graph line and the labels are those set by the user at setup. The toggle action operates to this rule: if All is ON then clicking any channel switches to just show that channel. If all the channels have been switched on by clicking on them then clicking on any one simply switches that channel off and leaves the others on. You cannot select to have no channels on. The last one on stays on if you choose to turn it off.



These show the number of graph points in total and showing on the current graph


These show the date and time range of the currently showing graph



The data pointer is set fully left when the screen loads. It can be moved by clicking anywhere on the bar length or dragging the Data Pointer indicator using the mouse. The indicator point can also be moved by using the] bracket to move it one data point at a time to the right or [bracket to move back in the time line. When the Data Pointer bar is selected by clicking on it the left and right keyboard arrows do the same as the [] brackets.

Moving the slider or clicking on the graph area causes a vertical Location Marker line to appear on the graph. The position of this Location Marker is copied on the Data Pointer bar.


The values of the channels corresponding to the position of the Location Marker or Data Point appear at the top of the screen. Only the channels selected to be showing on the graph display their values. The channels are coloured the same as the graph and are labelled as set by the user.



Transmitter channels

Temperature ranges

Data point time and date

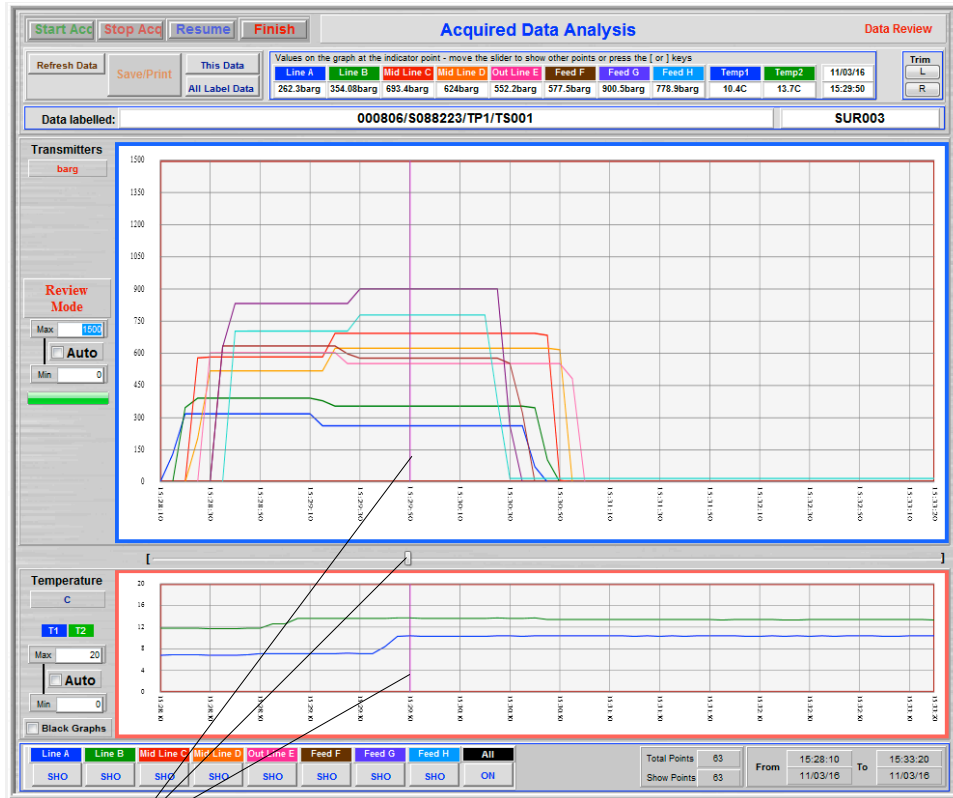

Location Markers and Data Point




Clicking Save/Print leads to the Saved Graph screen which allows saving and printing of the graph as a record of the test shown. The data range currently viewed and scales selected are used in the printing.

Saving and Printing the graphs can be prevented in the Levels section of the system. If the user has a Level access which prevents that the Save/Print button is not active.

Saved Graph Screen

The User's company name appears here. This is set in the Utilities menu
 This saves and prints this graph
 This stores this graph in the Graph file
 This exits this screen without saving the graph
 These are the data references for this graph
 The Customer name can be entered or altered here

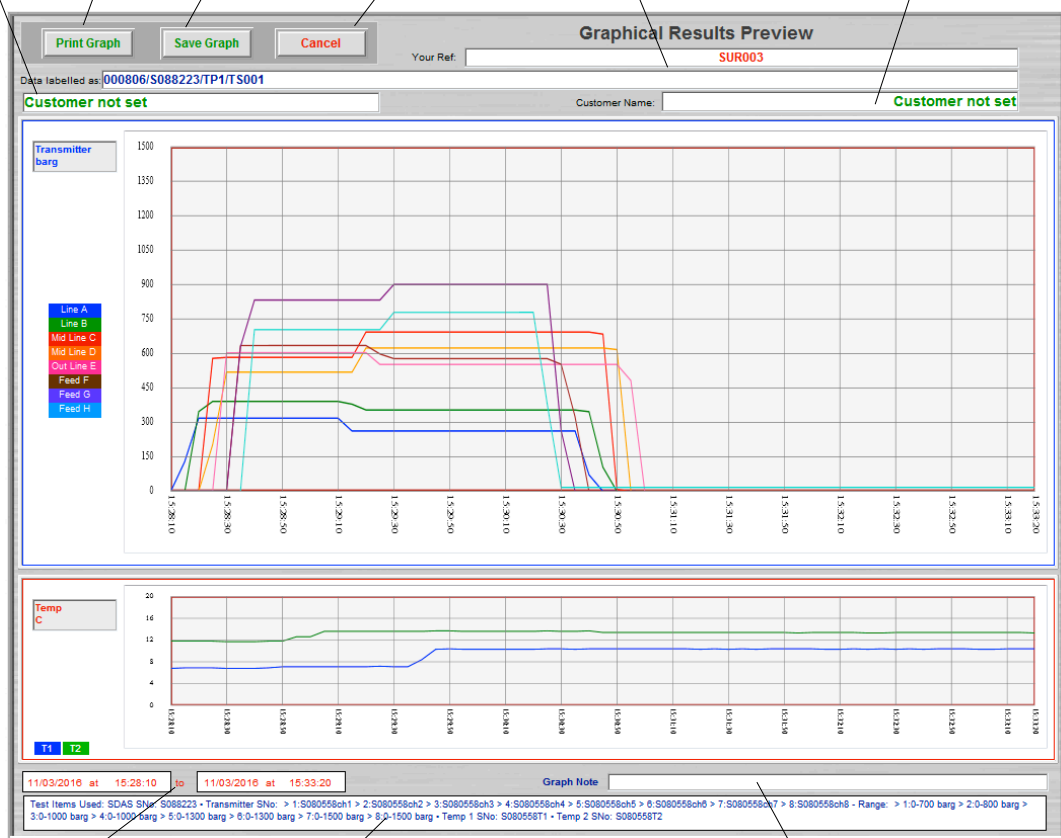




This shows the range of the graph with date and time

This is the equipment used for this test, SDAS serial number, transmitters serial numbers and ranges and the serial numbers of the temperature probes and any other info created with other options


This is an 80 character field which can be used to clarify why this graph is being saved or some other note

Printing Graphical Results


Clicking Print Graph on the previously displayed graph prints the following to the selected system printer. System print dialog boxes are displayed. If Print to Pdf is activated then a pdf is sent to the Save folder of the SDAS and these printing screens do not appear.

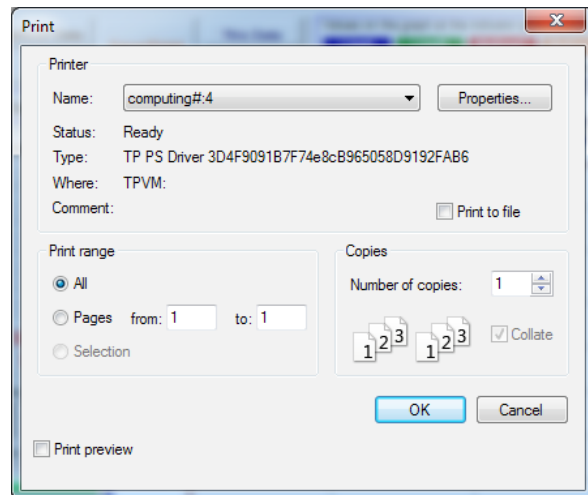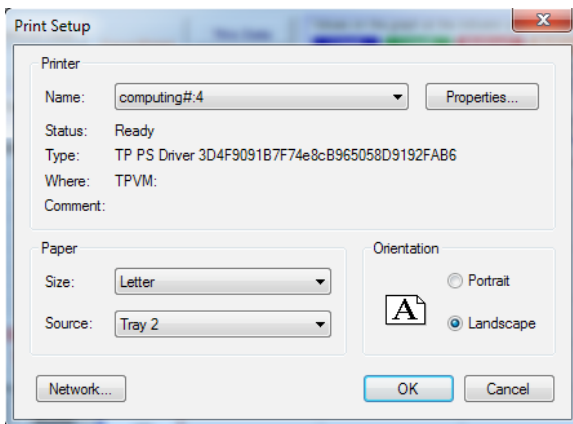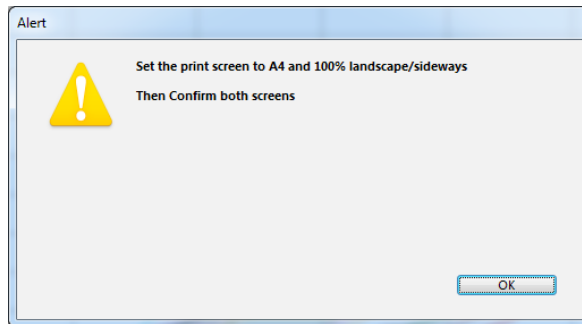

A print like this is produced on the printer or saved as pdf

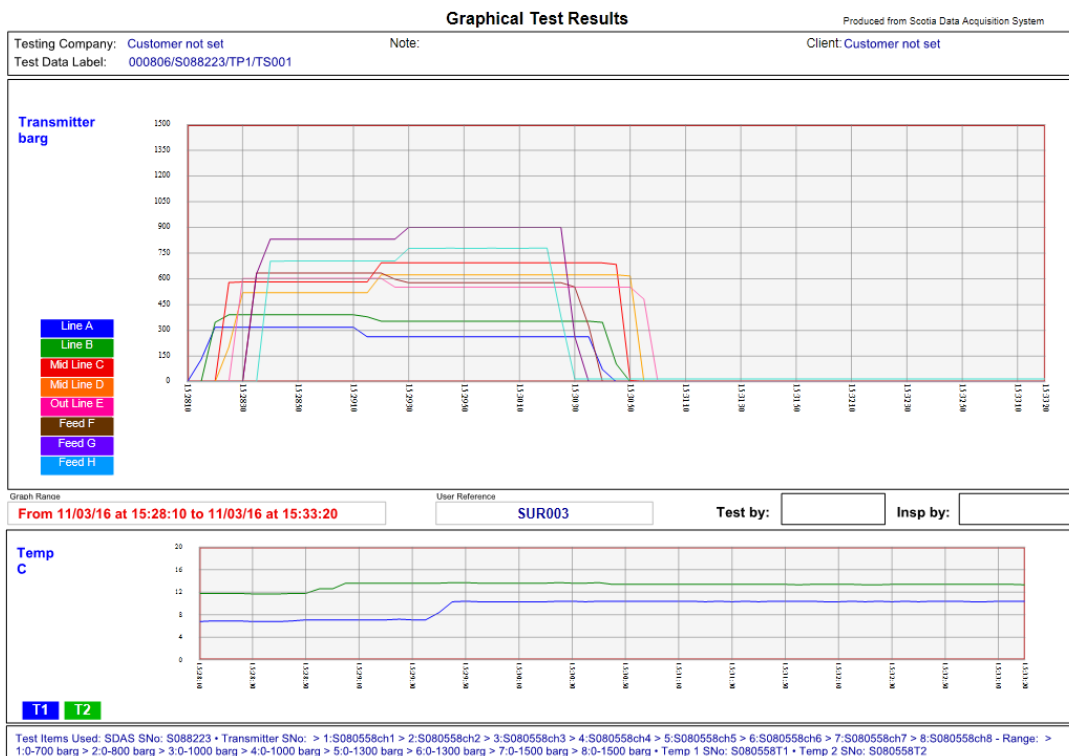


Review Stored Data

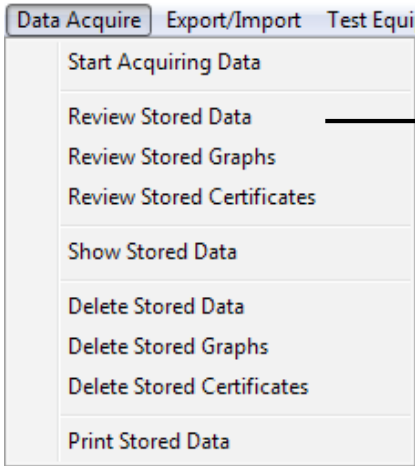


This routine allows currently stored data to be reviewed. Note that the data from one data label is regarded as unique. Only one set of this unique data can be shown on the graph screen at the same time. Choosing using the Data Label gives just one set of data but choosing by other methods can lead to more than one and further choosing may be necessary to get to only one.

Use Data Label


Choose the search type

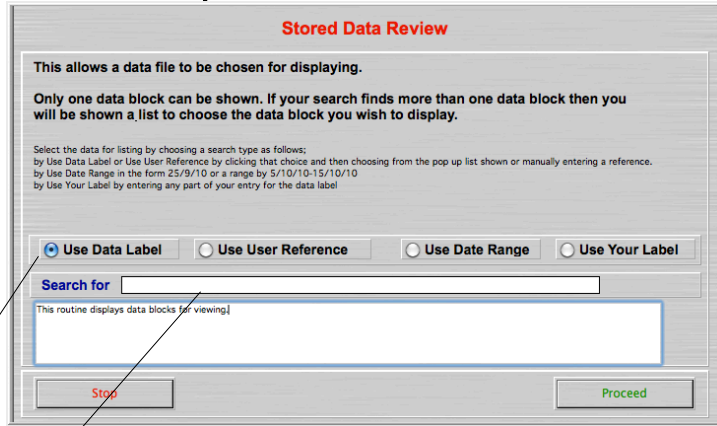

Click on the search type or the Search for entry to show this pick list if you have chosen the Use Data Label

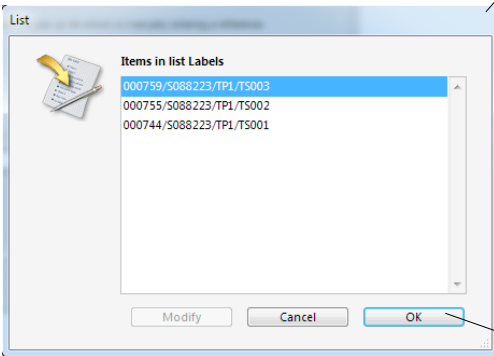


Click on the one required and then click OK to select this choice.

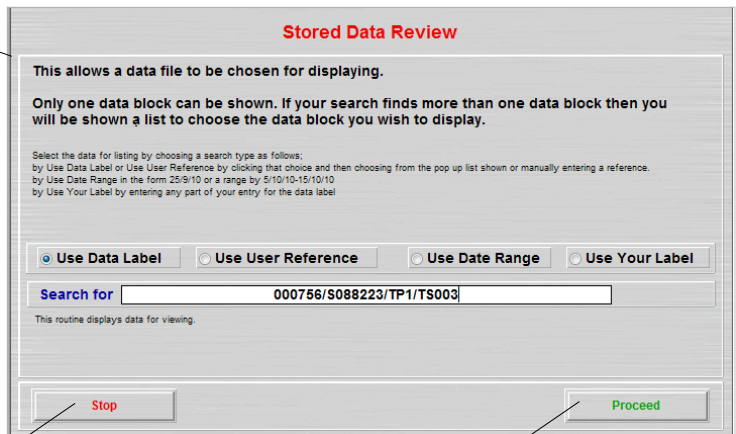


Click Stop to return to the start screen

Click Proceed to show the selected data

Use User Reference

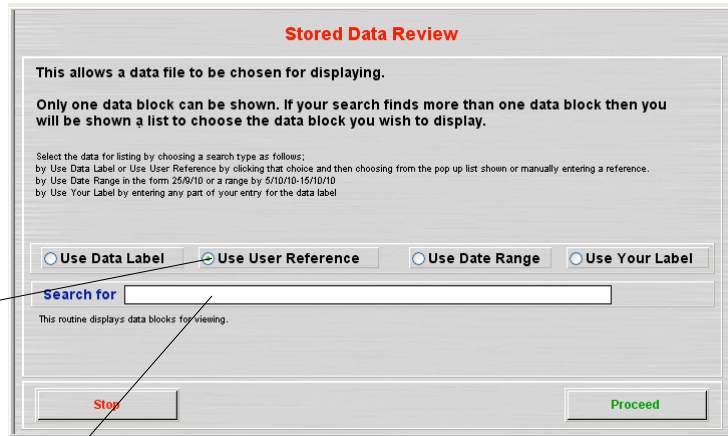


Choose search by User Reference

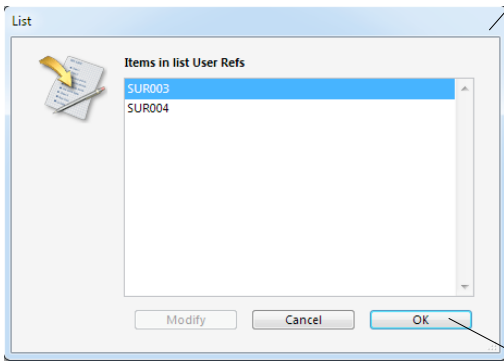

Click on the search type or the Search for entry to show this pick list if you have chosen the Use Data Label

Click on the one required and then click OK to select this choice.

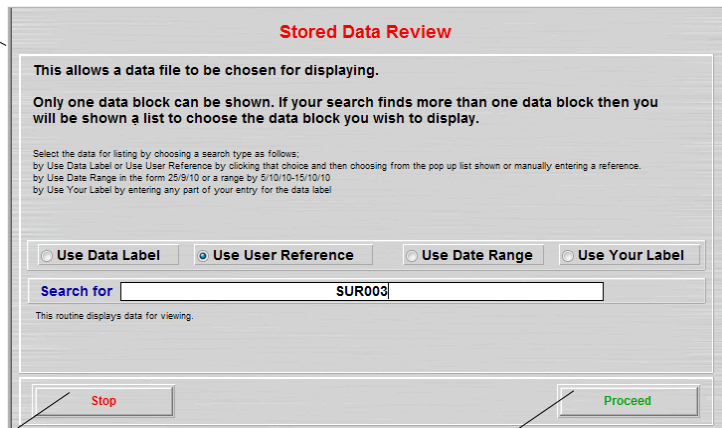


Click Stop to return to the start screen

Click Proceed to show the selected data

If only one data label set of data has this User Reference then the system will proceed to show this data on the Acquired Data Analysis screen. If more than one data label set of data has this User Reference then a list is shown for the user to make a selection. To aid selection data is added to the selection line. Each line has the Data Label > the User Reference > Test start date > Test start time > Test finish time

Choose from the list and then click proceed to show this data set on the Acquired Data Analysis screen

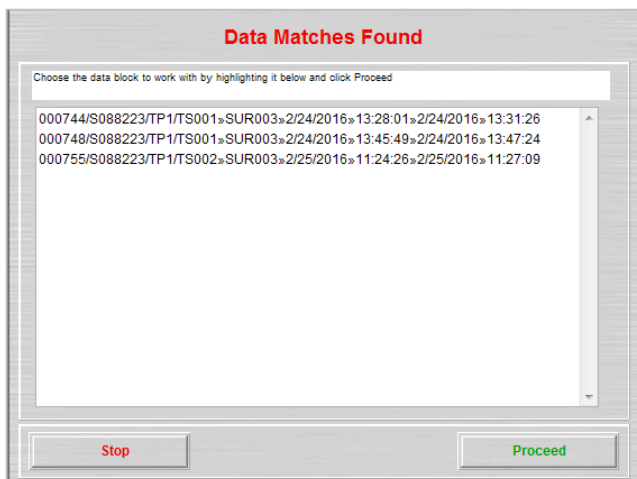

Use Date Range

Stored Data Review

This allows a data file to be chosen for displaying.

Only one data block can be shown. If your search finds more than one data block then you will be shown a list to choose the data block you wish to display.

Select the data for listing by choosing a search type as follows;
 by Use Data Label or Use User Reference by clicking that choice and then choosing from the pop up list shown or manually entering a reference.
 by Use Date Range in the form 25/9/10 or a range by 5/10/10-15/10/10
 by Use Your Label by entering any part of your entry for the data label

Use Data Label
 Use User Reference
 Use Date Range
 Use Your Label

Search for

This routine displays data blocks for viewing.

Choose search by Date Range

The cursor is placed in the answer field to allow the user to type the date or date range required. A single date is entered in the form DD/MM/YY (eg 20/02/16) but the system will accept single numbers or extended years - 20/2/2016 perhaps. A range of dates can be entered in the form 20/02/16-25/02/16 and any data labels within the range of the dates entered will be listed.

Stored Data Review

This allows a data file to be chosen for displaying.

Only one data block can be shown. If your search finds more than one data block then you will be shown a list to choose the data block you wish to display.

Select the data for listing by choosing a search type as follows;
 by Use Data Label or Use User Reference by clicking that choice and then choosing from the pop up list shown or manually entering a reference.
 by Use Date Range in the form 25/9/10 or a range by 5/10/10-15/10/10
 by Use Your Label by entering any part of your entry for the data label

Use Data Label
 Use User Reference
 Use Date Range
 Use Your Label

Search for

This routine displays data for viewing.

Click Stop to return to the start screen

Click Proceed to show the selected data

If only one data label set of data has this date or date range then the system will proceed to show this data on the Acquired Data Analysis screen. If more than one data label set of data has the date or range of dates then a list is shown for the user to make a selection. To aid selection data is added to the selection line. Each line has the Data Label > the User Reference > Test start date > Test start time > Test finish time

Choose from the list and then click proceed to show this data set on the Acquired Data Analysis screen

Data Matches Found

Choose the data block to work with by highlighting it below and click Proceed

000744/S088223/TP1/TS001»SUR003»24/02/2016»13:28:01»24/02/2016»13:31:26
000755/S088223/TP1/TS002»SUR003»25/02/2016»11:24:26»25/02/2016»11:27:09
000759/S088223/TP1/TS003»SUR004»25/02/2016»11:45:29»25/02/2016»11:46:41

Use Your Label

This routine searches the Label Data for any instance of the entry here. It can be used to search for a user initials, the data entered by the user for the end of the label and for the serial number of the SDAS where data is stored for more than one SDAS.

Choose search by Your Label

Stored Data Review

This allows a data file to be chosen for displaying.

Only one data block can be shown. If your search finds more than one data block then you will be shown a list to choose the data block you wish to display.

Select the data for listing by choosing a search type as follows:
 by Use Data Label or Use User Reference by clicking that choice and then choosing from the pop up list shown or manually entering a reference.
 by Use Date Range in the form 25/9/10 or a range by 5/10/10-15/10/10
 by Use Your Label by entering any part of your entry for the data label

Use Data Label Use User Reference Use Date Range Use Your Label

Search for

This routine displays data blocks for viewing.

The cursor is placed in the answer field to allow the user to type the data for the search. Any text can be entered. Any instance of the data entered will be found as a match. Be as specific as possible to avoid multiple matches.

Stored Data Review

This allows a data file to be chosen for displaying.

Only one data block can be shown. If your search finds more than one data block then you will be shown a list to choose the data block you wish to display.

Select the data for listing by choosing a search type as follows:
 by Use Data Label or Use User Reference by clicking that choice and then choosing from the pop up list shown or manually entering a reference.
 by Use Date Range in the form 25/9/10 or a range by 5/10/10-15/10/10
 by Use Your Label by entering any part of your entry for the data label

Use Data Label Use User Reference Use Date Range Use Your Label

Search for

This routine displays data blocks for viewing.

Click Stop to return to the start screen

Click Proceed to show the selected data

If only one data label set of data has this data then the system will proceed to show this data on the Acquired Data Analysis screen. If more than one data label set of data has the data entered then a list is shown for the user to make a selection. To aid selection data is added to the selection line. Each line has the Data Label > the User Reference > Test start date > Test start time > Test finish time

Choose from the list and then click proceed to show this data set on the Acquired Data Analysis screen


Data Matches Found

Choose the data block to work with by highlighting it below and click Proceed

000744/S088223/TP1/TS001»SUR003»24/02/2016»13:28:01»24/02/2016»13:31:26
000755/S088223/TP1/TS002»SUR003»25/02/2016»11:24:26»25/02/2016»11:27:09
000759/S088223/TP1/TS003»SUR004»25/02/2016»11:45:29»25/02/2016»11:46:41

Data Analysis Screen

The data for this Data Label is then selected and displayed graphically

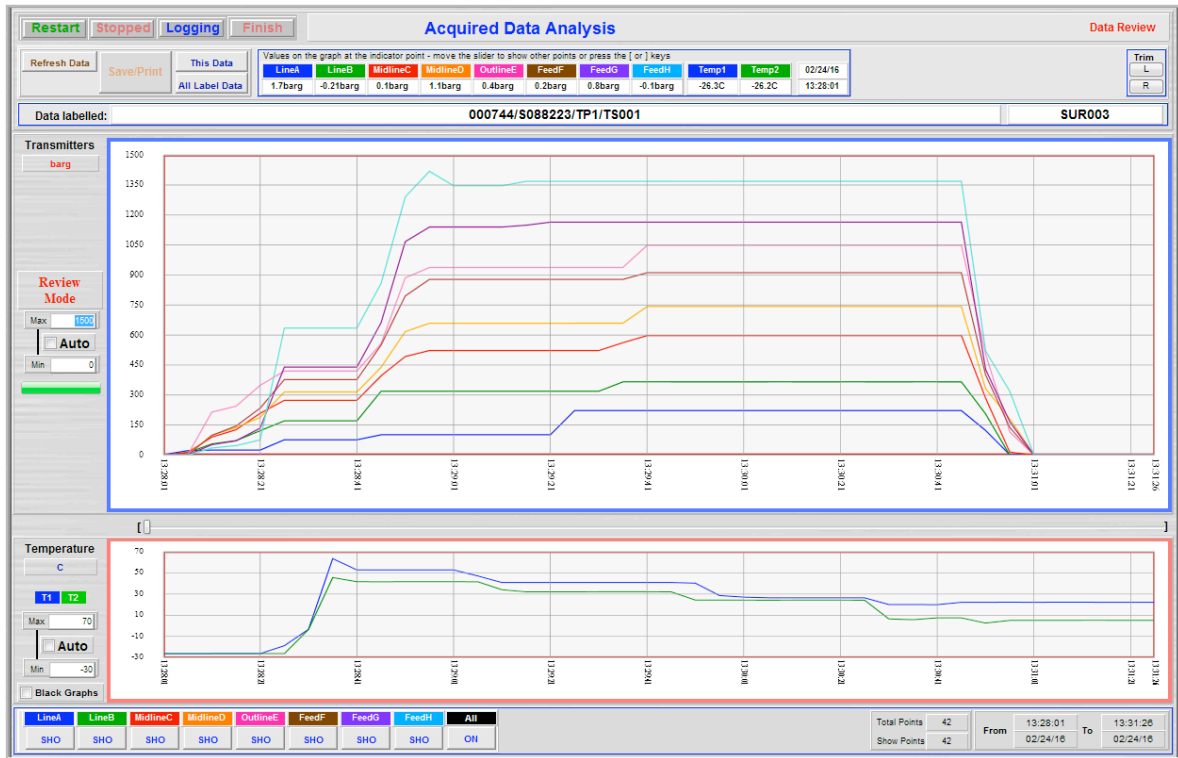

The screen above will be divided into parts in order to describe the various functions


L-R Trimmer Bar

This restarts acquiring if it has been stopped

This returns to the acquiring screen

Values shown here when the screen opens are for the left side of the graphs

L-R trimming - Used in conjunction with the Location marker - clicking L or R will move the left or right end of the graph up to the Location Marker.

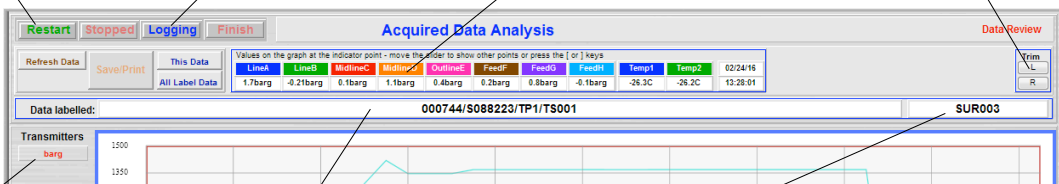

This shows the Transmitter units. If more than one unit is being graphed then this shows 'various' and the graph shown is in percentage

Clicking here gives a pop up list of the saved data files labels. Selecting from the list will load that file into the Review graphs below even if acquiring is continuing to the original file.

Clicking here gives a pop up list of the saved User labels. Selecting from the list will load that file into the Review graphs below even if acquiring is continuing to the original file.

Stored Data Values

This resets the graph to show all the current label data stored


This is the current mode identifier

While Auto is checked the graph will autorange in the values axis to best fit all currently shown graphed values. If unchecked the graph range is set by typing values into the Max and Min boxes.

This is a visual percentage indicator of the amount of data showing for the current data label.

This shows the colour coding of the graphed temperatures

While Auto is checked the graph will autorange in the values axis to best fit all currently shown graphed values. If unchecked the graph range is set by typing values into the Max and Min boxes.

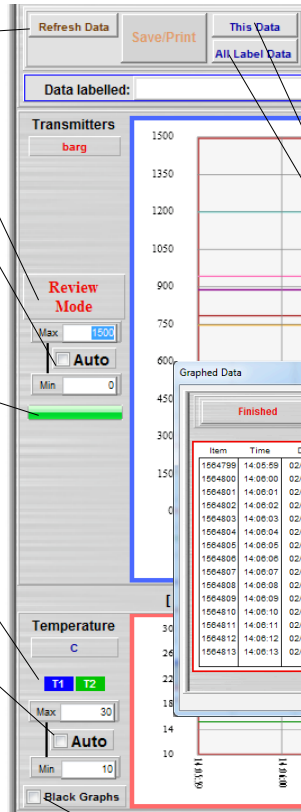


Clicking the This Data or All Label Data gives a floating display of the current data label values. 'This Data' shows the data currently graphed and 'All Label Data' shows all the data saved for this label. The list can be scrolled and the floating display can be moved around the screen if required. The graph loads with the start and finish values being either the range of the currently showing graph or all the label data. It can be used to set the Graphs to a new range of values by clicking on the required start value and then clicking on the required finish value on the listed values. The from and to values update as you do so. You can reselect by repeating this action. Clicking Regraph will select this range for graphing. Clicking Finished will just restore the current graphing range.

If checked this sets the graph to display on a black background

Channel Selection Buttons



These control the channels displayed - clicking a channel control toggles it from showing SHO to hidden HID. Any channel not selectable is shown as disabled DIS and does not show on the graph. 'All' allows all channels not set to DIS to be selected as showing SHO. The colours on the channel labels match the colour of the graph line and the channel labels are those set by the user at setup.

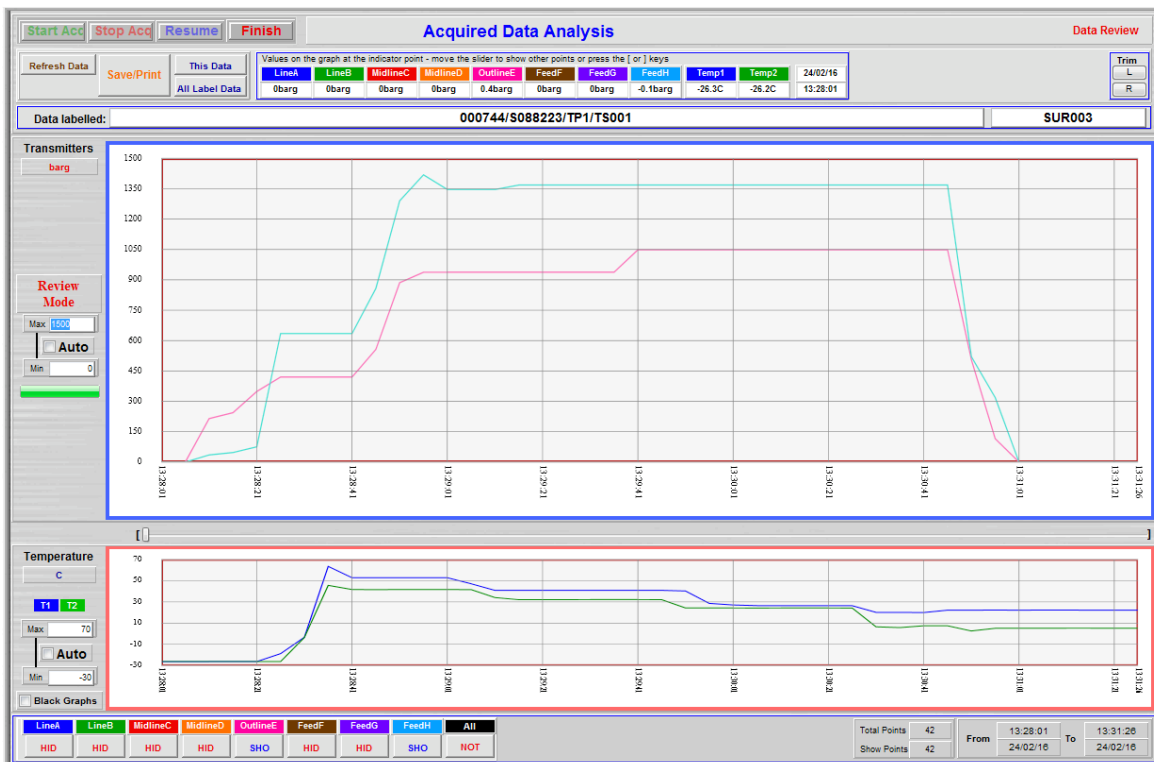


A toggling system is set up in the following way. If all channels are showing - either from just opening the screen or by clicking the All button then clicking a channel just selects that channel SHO and other active channels go HID. In all other ways clicking a channel at SHO sets it to HID and one at HID changes it to SHO. Channels 5 and 8 have been set to SHO here and only those values are showing on the graph area.

The temperature channels cannot be toggled off and on. There is an option to not show temperature 2 given at start up


Location Marker and Data Pointer Bar

Once data pointer is moved from fully left the values of the visible channels corresponding to the position of the data pointer appear at the top of the screen. Only the channels showing on the graph display their values. The channels are coloured the same as the graph and are labelled as set by the user. Moving the Data Pointer back fully left causes this part of the display to disappear again.




The data pointer is set fully left when the screen loads. It can be moved by clicking anywhere on the bar length or dragging the Data Pointer indicator using the mouse. The indicator point can also be moved by using the] bracket to move it one data point at a time to the right or [bracket to move back in the time line. When the Data Pointer bar is selected by clicking on it the left and right keyboard arrows do the same as the [] brackets.

Clicking on the graph area causes a vertical Location Marker line to appear on the graph. The position of this Location Marker is copied on the Data Pointer bar.

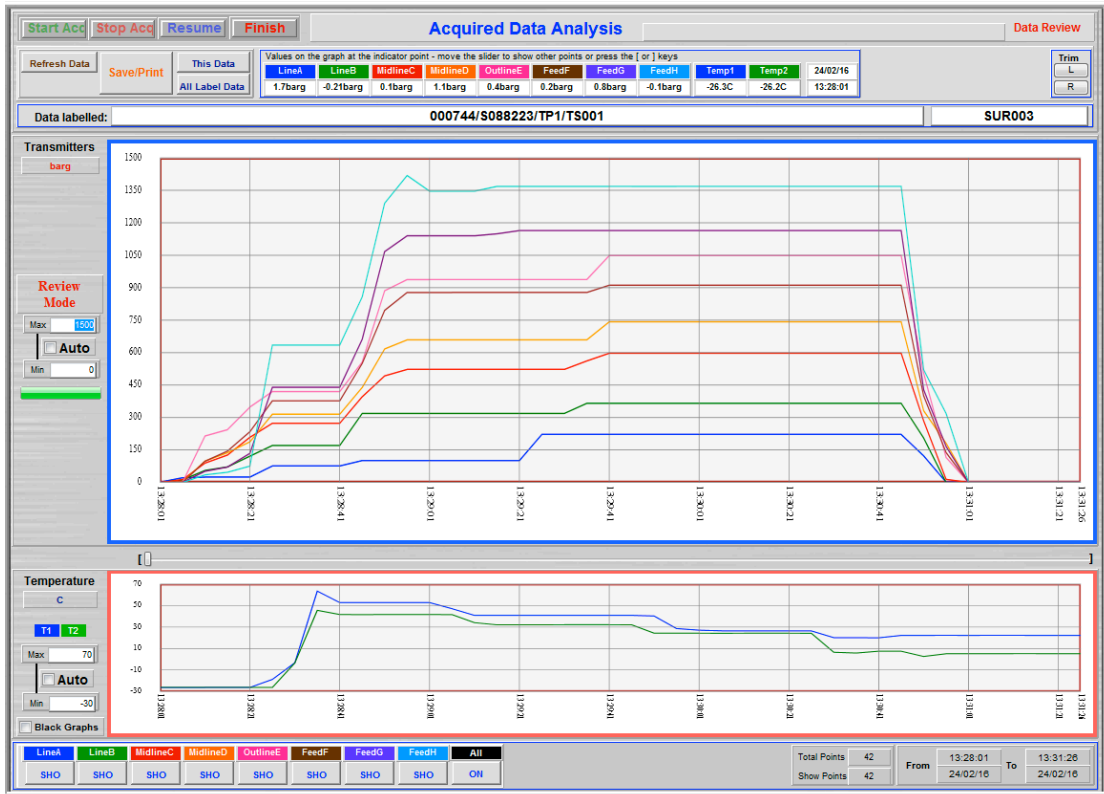

Only the channels currently showing have their values shown here




Transmitter channels

Temperature ranges

Data point time and date

Time Scale Indicator



These show the number of graph points in total and showing on the current graph

These show the date and time range of the currently showing graph

Save/Print button



This leads to the saved graph screen which allows saving and printing of the graph as a record of the test shown. The data range currently viewed and scales selected are used in the printing. Set up the graph you wish to save and/or print first.

Saved Graph Screen

The User's company name appears here. This is set in the Utilities menu


This saves and prints this graph

This stores this graph in the Graph file

This exits this screen without saving the graph

These are the data references for this graph

The Customer name can be entered or altered here

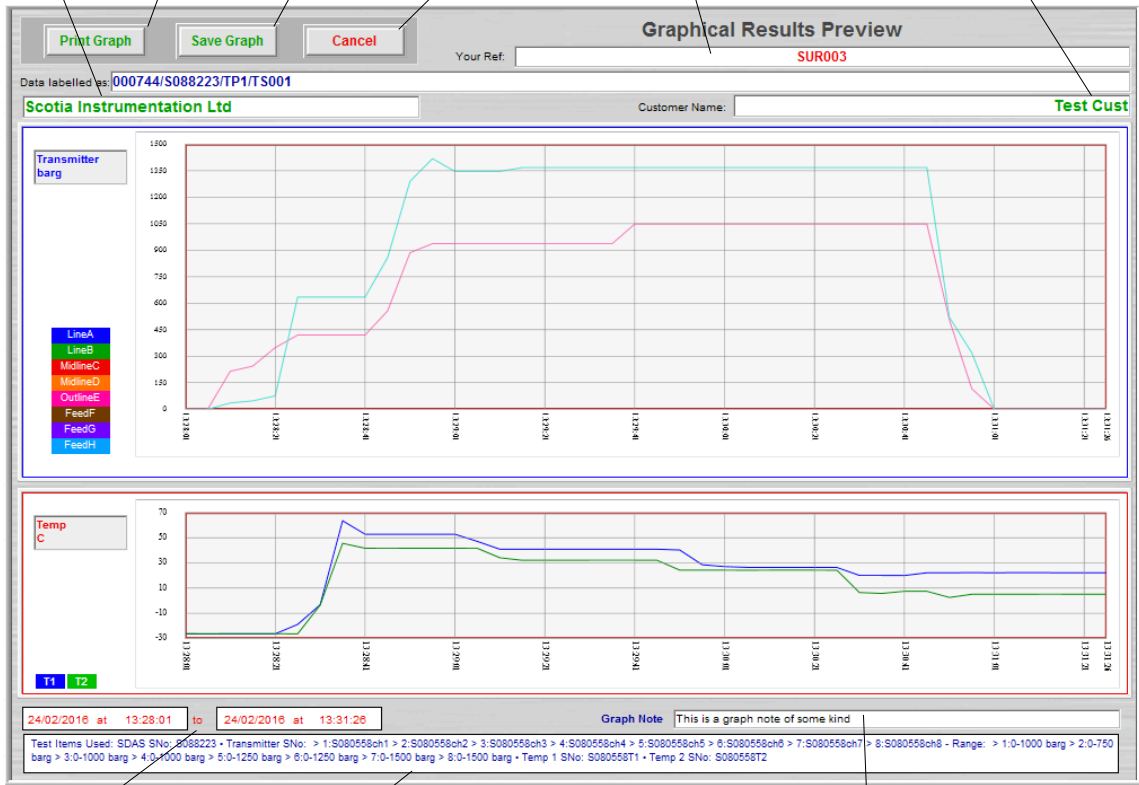

This shows the range of the graph with date and time


This is the equipment used for this test, SDAS serial number, transmitters serial numbers and ranges and the serial numbers of the temperature probes


This gives an 80 character field which can be used to clarify why this graph is being saved or some other note

Printing Graphical Results


Clicking Print Graph on the previously displayed graph prints the following to the selected system printer. System print dialog boxes are displayed. If pdf printing is chosen then a pdf is saved to the saving folder and the print screens do not show.

A guidance screen is shown to advise the printing format to display the graph properly on the printer paper

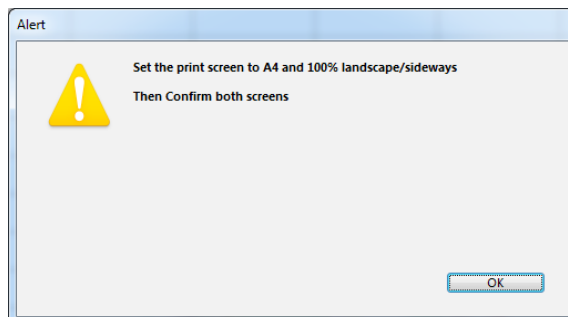


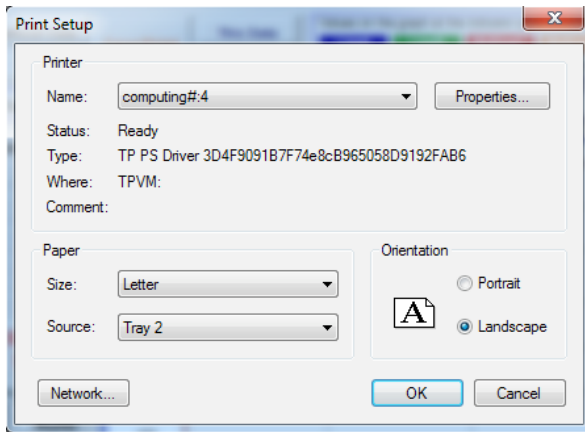

Set the values on the print settings screens and confirm both. Names and settings may vary for different printers

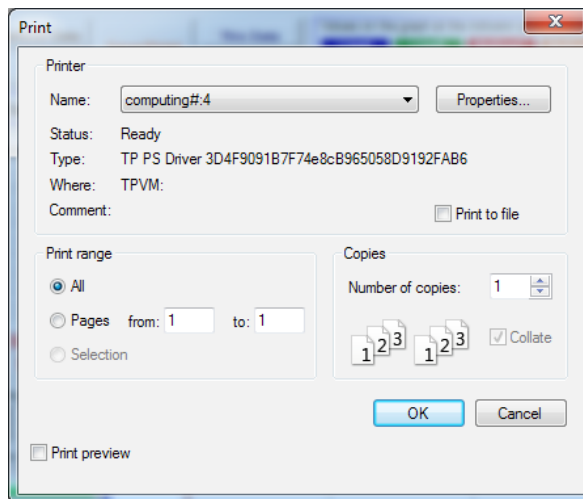


Printed Graphical Results

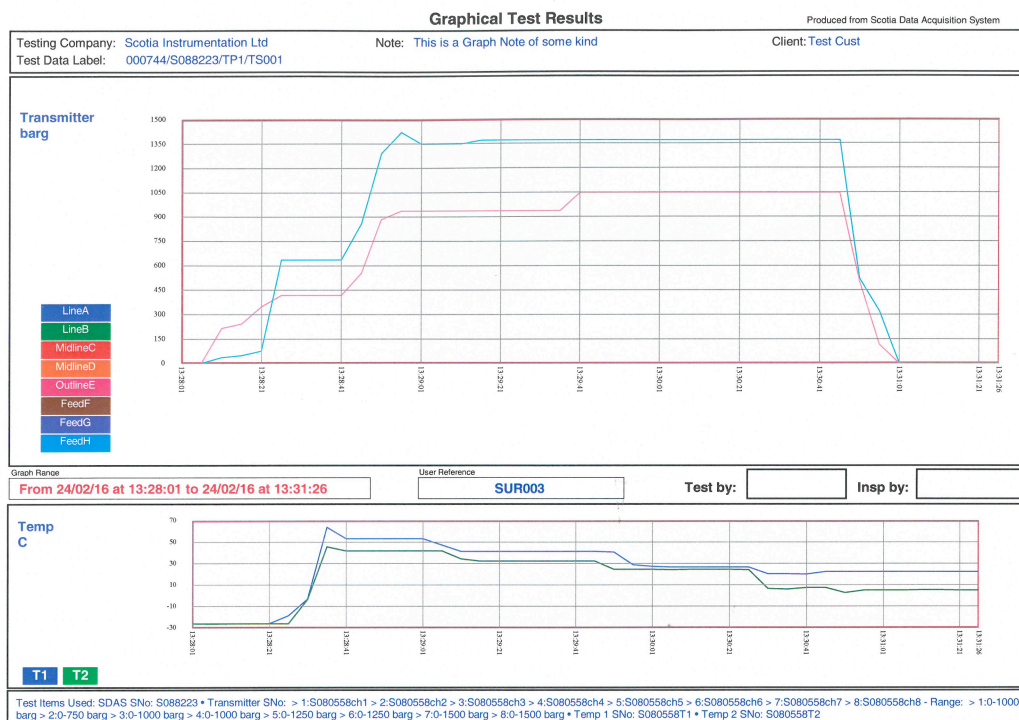


Once this is printed the user is returned to the Data Analysis screen

Review Stored Graphs

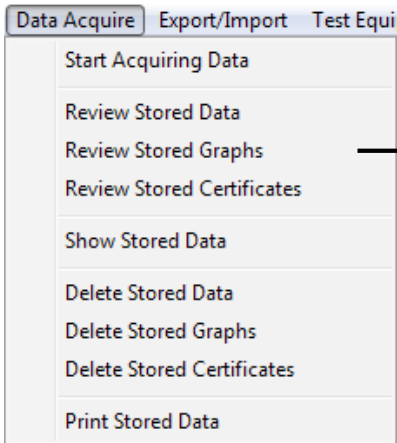



This routine allows currently stored graphs to be reviewed. Note that these are stored under their data label name and several graphs can be stored from the same data label. If more than one match is found for the search initiated then the results are listed for choosing the correct one.

Choose the search type

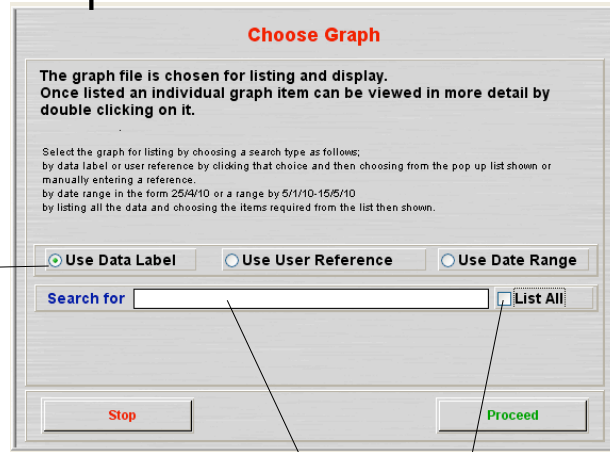

Checking this box selects all the stored graphs

Click on the search type and the list of currently stored graphs Data Labels are shown. Click on the one required and then click OK to select this data label. Note that more than one graph may be stored for one label. The list is in reverse order so the most recent should be at the top. Clicking List All will show all stored Graphs.

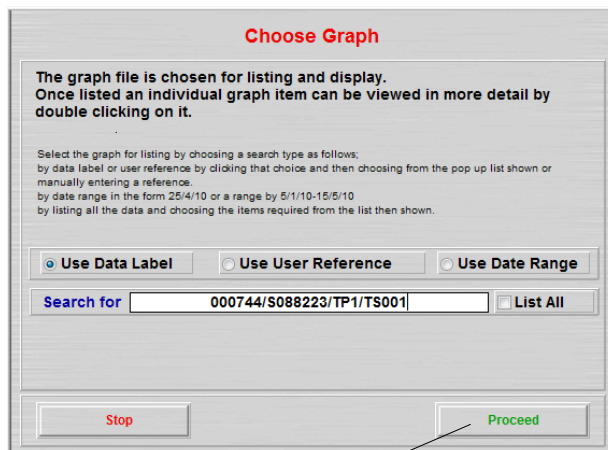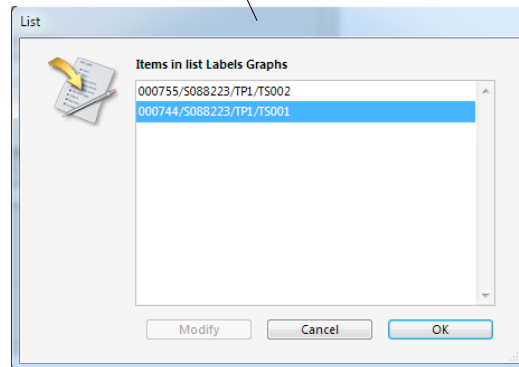

This Label is entered as the choice. Click confirm to proceed or click on the Search For entry point to choose again.

Stored Graph Listing

The stored graphs are then listed. The graphs are listed whether one is found or many.

Graph Listing

Select from the list below by clicking - shift clicking or control clicking. Reduce the selection to those required by clicking Reduce Selection. View Graphs by Double-clicking on the one required. Print the Graphs listed by clicking Print Selection.

ID Graph	Data Label	User Reference	Start Date	Start Time	Finish Date	Finish Time	Origination
42	000744/S088223/TP1/TS001	SUR003	24/02/16	13:28:01	24/02/16	13:31:26	Created>25/02/2016
43	000744/S088223/TP1/TS001	SUR003	24/02/16	13:28:01	24/02/16	13:31:26	Created>25/02/2016
44	000744/S088223/TP1/TS001	SUR003	24/02/16	13:28:01	24/02/16	13:31:26	Created>25/02/2016
45	000744/S088223/TP1/TS001	SUR003	24/02/16	13:28:01	24/02/16	13:31:26	Created>25/02/2016
41	000744/S088223/TP1/TS001	SUR003	24/02/16	13:28:01	24/02/16	13:31:26	Created>25/02/2016

These sort the column above them up or down

This completes this routine

This completes this routine

This reduces the selection to only the graphs chosen. Highlight those required by clicking, shift clicking or control clicking before clicking this button.

This prints all the graphs listed above after showing the Print Settings screens. Note that all the listed graphs will be printed if you do not select the one or ones required and then click Reduce Selection. You need to reduce the listed selection to ONLY the graphs you wish to print.

Double clicking on any listed Graph displays it in full

Graph Results Display

This saves changes to the graph and returns to the Stored Graph Listing


This prints the graph and saves changes to the graph and returns to the Stored Graph Listing

This returns to the Stored Graph Listing without saving any changes

These move through the list of graph captures. They only display if the move is possible

These are the data references for this graph

If the customer name has been saved with the Graph capture it appears here. It can be entered or altered here.

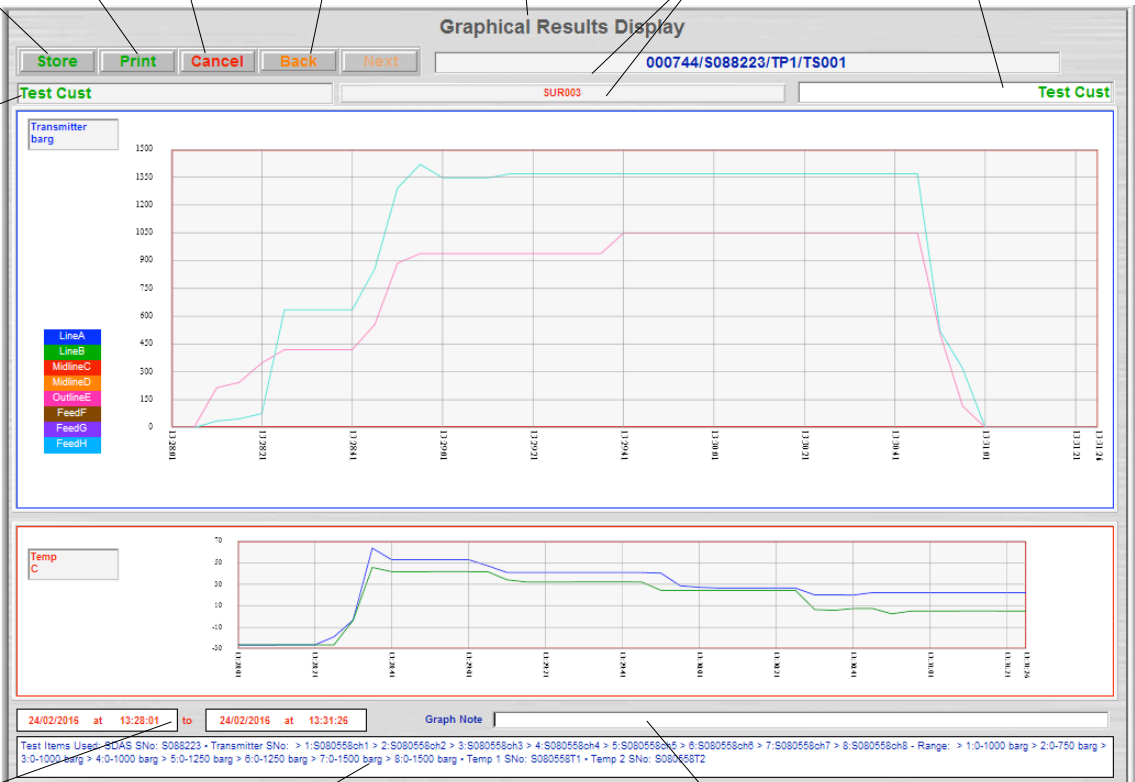

If the user company name has been saved with the Graph capture it appears here


In order to hold the text proportions of the picture of these graphs the graphs are sized proportionately and may not fill the available space on the screen

This shows the range of the graph with date and time


This is the equipment used for this test, SDAS serial number, transmitter serial numbers and ranges and the serial numbers of the temperature probes

This gives an 80 character field which can be used to clarify why this graph is being saved or some other note


Review Stored Certificates

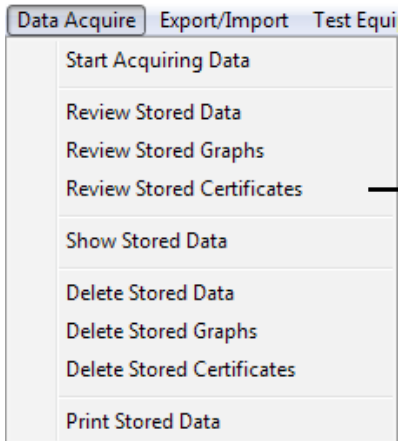


This option allows the creation of a certificate for a test. This is covered in the options section of this manual. If this is not enabled then this alert screen appears.

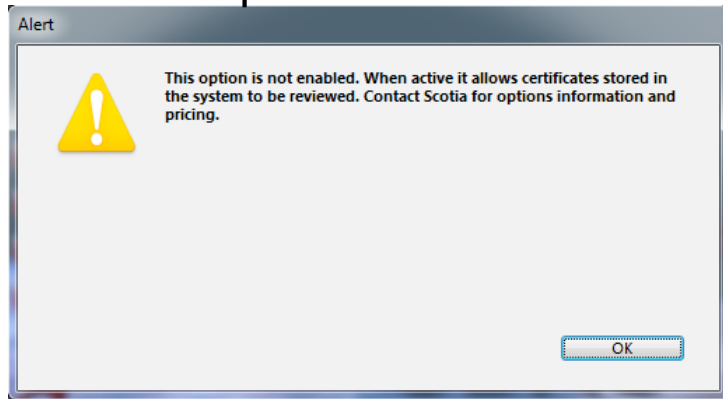

Show Stored Data

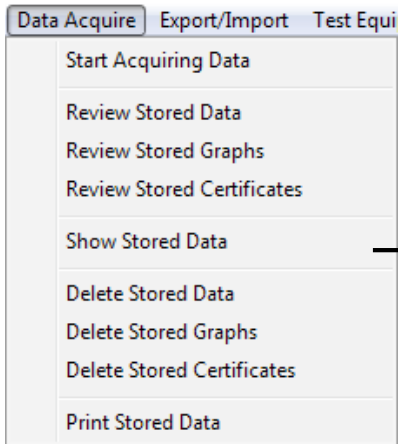


This routine allows currently stored data values to reviewed.

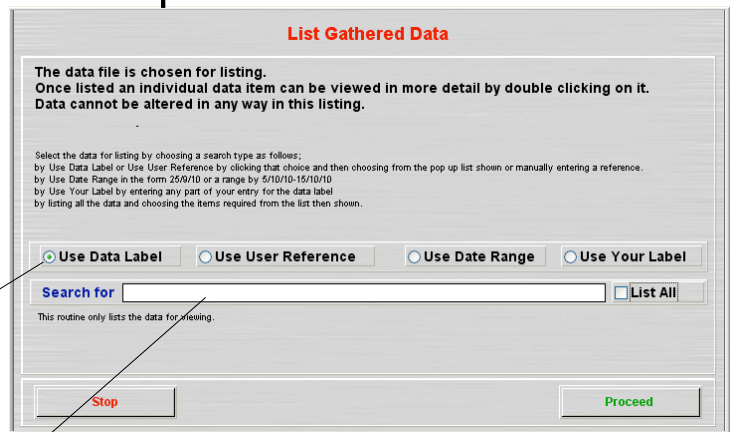

Choose the search type


Click on the search type or the Search for entry to show this pick list if you have chosen the Use Data Label

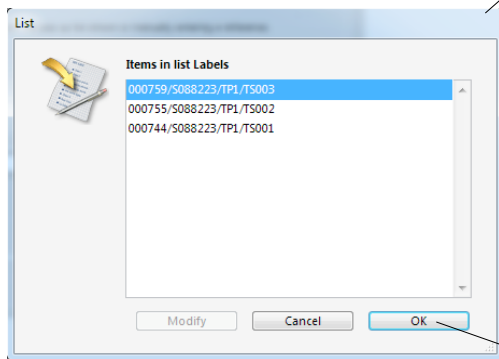

Choosing to search by User Reference, Data Range or Your Label will show all the matching data events for that search. This can involve several Data Labels' data. Checking the List All box will show all the stored data.

If the number of data items exceed the limit for displaying - default is 10,000 - then the data must be displayed either in blocks of 10,000 or by sampling the data to the limit of 10,000. The user is asked to choose which if this is the case.

Click on the one required and then click OK to select this choice.

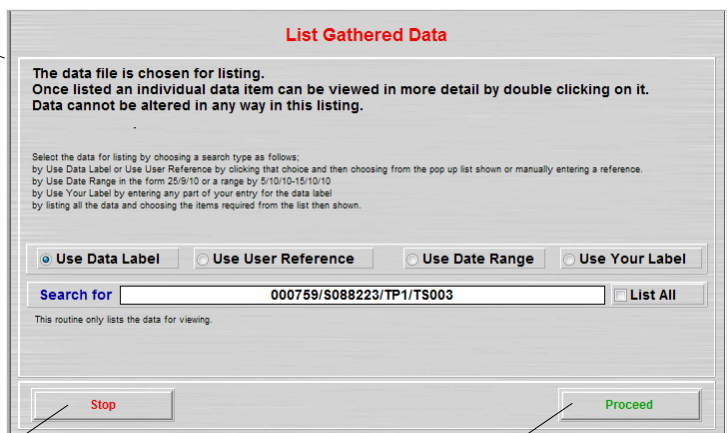

Click Stop to return to the start screen

Click Proceed to show the selected data

Listing of Data Acquired

The stored data items are then listed.

Data Acquired

Select from the list below by clicking, shift-clicking, control-clicking and then use Reduce Selection to leave just the records required on the list. Control-A selects all the data records. When the data is listed in blocks then Back and Next moves between blocks.

Data Label	User Reference	Data ID	Date	Time	Temp1	Temp2	Counters
000759/S088223/TP1/TS003	SUR004	1565363	25/02/16	11:45:29	10.10	39.00 C	OFF Counts OFF Counts OFF Counts
Data 02/25/16	1-S080558ch1	230.1 barg	159.95 barg	484.6 barg	570 barg	404.4 barg	614.6 barg 994.8 barg 765.7 barg
000759/S088223/TP1/TS003	SUR004	1565364	25/02/16	11:45:30	10.10	39.00 C	OFF Counts OFF Counts OFF Counts
Data 02/25/16	2-S080558ch2	230.1 barg	159.94 barg	484.6 barg	570 barg	404.4 barg	614.6 barg 994.8 barg 765.7 barg
000759/S088223/TP1/TS003	SUR004	1565365	25/02/16	11:45:31	10.10	39.00 C	OFF Counts OFF Counts OFF Counts
Data 02/25/16	3-S080558ch3	230.1 barg	159.95 barg	484.6 barg	570 barg	404.4 barg	614.6 barg 994.8 barg 765.7 barg
000759/S088223/TP1/TS003	SUR004	1565366	25/02/16	11:45:32	10.10	39.00 C	OFF Counts OFF Counts OFF Counts
000759/S088223/TP1/TS003	SUR004	1565377	25/02/16	11:45:43	1.20	22.00 C	OFF Counts OFF Counts OFF Counts
Data 02/25/16	7-S080558ch7	230.3 barg	159.94 barg	484.6 barg	570 barg	404.4 barg	614.6 barg 994.8 barg 765.7 barg
000759/S088223/TP1/TS003	SUR004	1565378	25/02/16	11:45:44	1.90	21.90 C	OFF Counts OFF Counts OFF Counts

These sort the column above them up or down

This completes this routine

This returns the listing to the original list if Reduce Selection has been used.

This reduces the selection to only those selected. Select by clicking - shift clicking or control clicking

This completes this routine

If the data has been segmented to display in 10,000 blocks then next and back buttons appear here to allow moving between blocks

Double clicking on a listed item shows more detail. Note that data cannot be altered in any way.

The appearance of this screen may change with different SDAS options

The labeling of each data field shows the type of data

The labels set by the user at the start of logging a test are shown here

Medium and A/D Label are used with other options

Imported data status is labelled differently from gathered data

This is the code for the options set for this data set

If counters are active their values show here. -1 is counter off

Data Item

ID: 1565363

Data Label: 000759/S088223/TP1/TS003

User Ref: SUR004

Date: 25/02/2016 Time: 11:45:29

Transmitter S/No: 1-S080558ch1 Range: 1-0-1000

Offsets:

LineA	230.1 barg	0
LineB	159.95 barg	0
MidlineC	484.6 barg	0
MidlineD	570 barg	0
OutlineE	404.4 barg	0
FeedF	614.6 barg	0
FeedG	614.6 barg	0
FeedH	765.7 barg	0

Temperature 1: 10.1 C

Temperature 2: 39 C

Medium:

A/D Label: Label not set

Status: Data 02/25/16

Options Set: 2359299

Counter 1: -1 Counts

Counter 2: -1 Counts

Counter 3: -1 Counts

Sig Figs set: 5/5

Channels Set: 1111111

Temp Probe 1: S080558T1

Temp Probe 2: S080558T2


The serial number and range of the 8 transmitters of the channels are stored successively in each data item. The channel number is shown before each.

The zero offset at the start of this test are shown here for each channel


If the option for significant figures is active then any change to default is stored here

This shows the channel settings 1 is on and 2 and 3 are disabled


Delete Stored Data

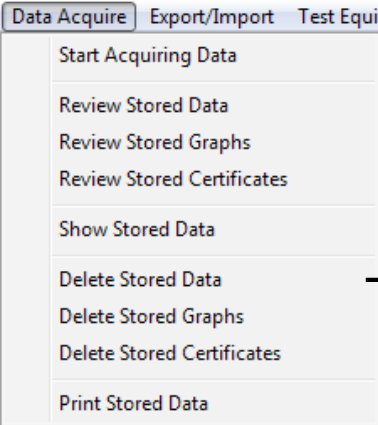

This routine deletes data from the SDAS. Access to this routine is restricted and normal users will get this screen when they choose this menu item.

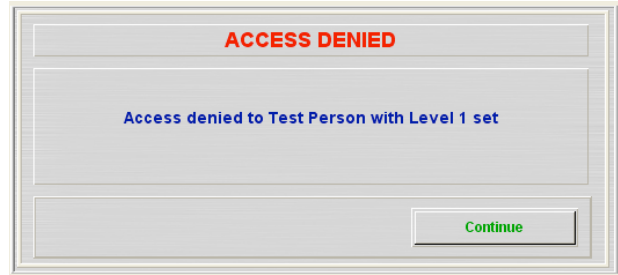


For users with a level access which enables them to proceed this screen is shown

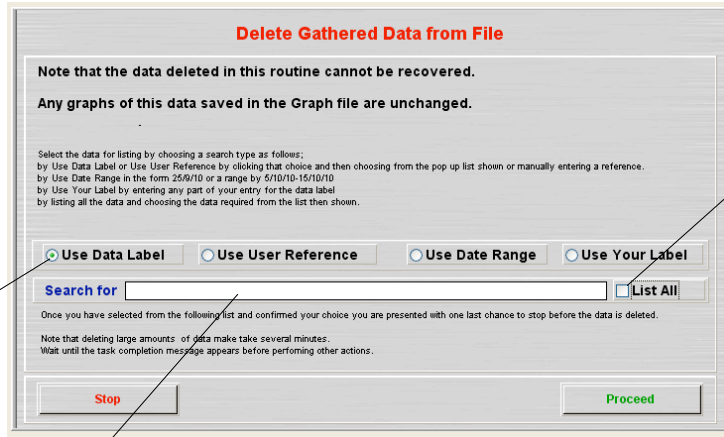

Choose the search type

Checking this box selects all the stored data

Click on the search type or the Search for entry to show this pick list if you have chosen the Use Data Label

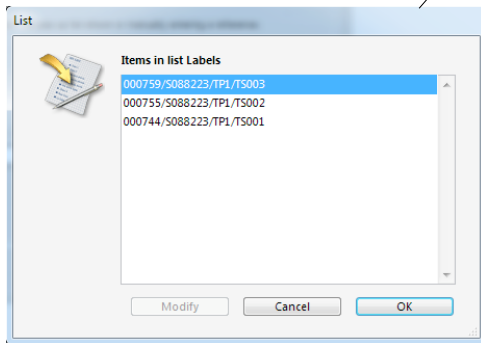

Choosing to search by User Reference, Data Range or Your Label will show all the matching data events for that search. This can involve several Data Labels' data. Checking the List All box will show all the stored data.

If the number of data items exceed the limit for displaying - default is 10,000 - then the data must be displayed either in blocks of 10,000 or by sampling the data to the limit of 10,000. The function of this routine - to delete all the found data - is not affected by this as it will delete all the data chosen not just those displayed.

Choose from the list presented and click OK to proceed.



This Label is entered as the choice. Click confirm to proceed or click on the Search for entry point to choose again.

Listing of Data for Deletion

The stored data items are then listed.

Data Acquired

Select from the list below by clicking, shift-clicking, control-clicking and then use Reduce Selection to leave just the records required on the list. Control-A selects all the data records. When the data is listed in blocks then Back and Next moves between blocks.

Data Label	User Reference	Data ID	Date	Time	Temp1	Temp2	Counters		
000755/S088223/TP1/TS002	SUR003	1564851	25/02/16	11:24:26	-26.20	180.00 C	OFF Counts	OFF Counts	OFF Counts
Data 02/25/16 1.S080556ch1	1.7 barg	-0.24 barg	0.2 barg	1.1 barg	0.5 barg	0.3 barg	0.5 barg	0 barg	
000755/S088223/TP1/TS002	SUR003	1564852	25/02/16	11:24:27	-26.10	180.10 C	OFF Counts	OFF Counts	OFF Counts
Data 02/25/16 2.S080556ch2	1.7 barg	-0.24 barg	0.2 barg	1.1 barg	0.5 barg	0.3 barg	0.5 barg	0 barg	
000755/S088223/TP1/TS002	SUR003	1564853	25/02/16	11:24:28	-26.10	180.10 C	OFF Counts	OFF Counts	OFF Counts
Data 02/25/16 3.S080556ch3	1.7 barg	-0.24 barg	0.2 barg	1.1 barg	0.5 barg	0.3 barg	0.5 barg	0 barg	
000755/S088223/TP1/TS002	SUR003	1564854	25/02/16	11:24:29	-26.20	180.00 C	OFF Counts	OFF Counts	OFF Counts
Data 02/25/16 4.S080556ch4	1.7 barg	-0.24 barg	0.2 barg	1.1 barg	0.5 barg	0.3 barg	0.5 barg	0 barg	
000755/S088223/TP1/TS002	SUR003	1564855	25/02/16	11:24:30	-26.30	180.00 C	OFF Counts	OFF Counts	OFF Counts
Data 02/25/16 6.S080556ch5	1.7 barg	-0.23 barg	0.2 barg	1.1 barg	0.5 barg	0.3 barg	0.5 barg	0 barg	
000755/S088223/TP1/TS002	SUR003	1564855	25/02/16	11:24:40	-26.30	120.70 C	OFF Counts	OFF Counts	OFF Counts
Data 02/25/16 7.S080556ch7	1.7 barg	-0.23 barg	0.2 barg	1.1 barg	0.5 barg	0.3 barg	0.5 barg	0 barg	
000755/S088223/TP1/TS002	SUR003	1564856	25/02/16	11:24:41	-26.20	112.50 C	OFF Counts	OFF Counts	OFF Counts
Data 02/25/16 8.S080556ch8	1.7 barg	-0.24 barg	0.2 barg	1.1 barg	0.5 barg	0.3 barg	0.5 barg	0 barg	

This completes this routine without deleting


This returns the listing to the original list.

This reduces the selection to only those selected. Select by clicking - shift clicking or control clicking. Only those finally listed will be deleted.


If the data has been segmented to display in 10,000 blocks then next and back buttons appear to allow moving between blocks

This proceeds with this selection to deletion


The user is asked to confirm this action

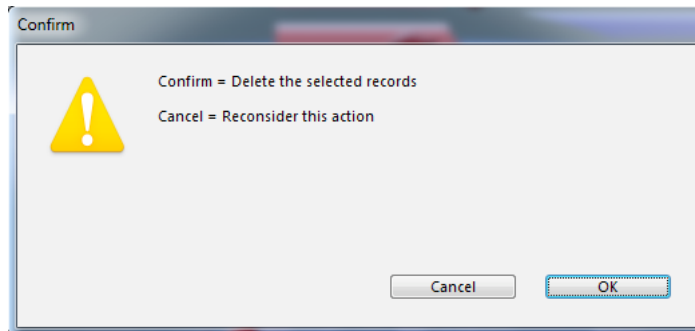


If OK clicked then the deletion routine proceeds and the following screen confirms completion

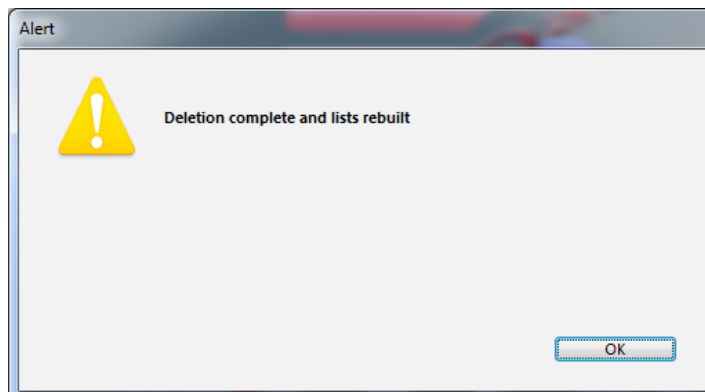


Delete Stored Graphs

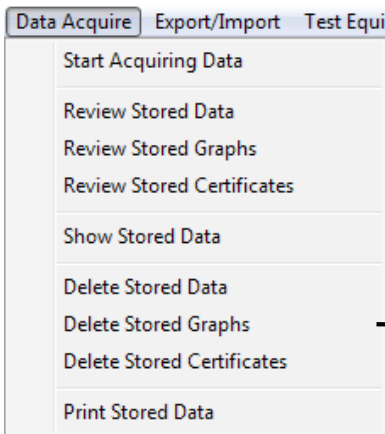

This routine deletes data from the SDAS. Access to this routine is restricted and normal users will get this screen when they choose this menu item.

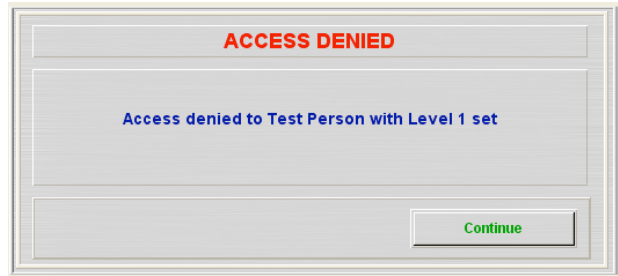


For users with a level access which enables them to proceed this screen is shown

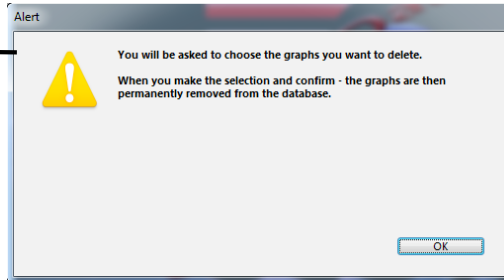


Click on the search type and the list of currently stored graphs data or user labels are listed. Click on the one required and then click OK to select this data label. Note that more than one graph may be stored for one label. Choosing Date Range allows entry of a date in the form 20/2/16 or a range of dates as 20/2/16-25/2/16. Clicking List All will show all stored Graphs.

Choose the search type

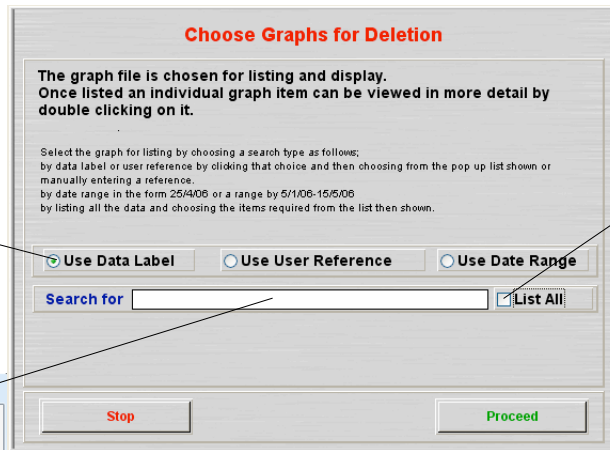


Checking this box selects all the stored data

Click on the search type or the Search for entry to show this pick list if you have chosen the Use Data Label

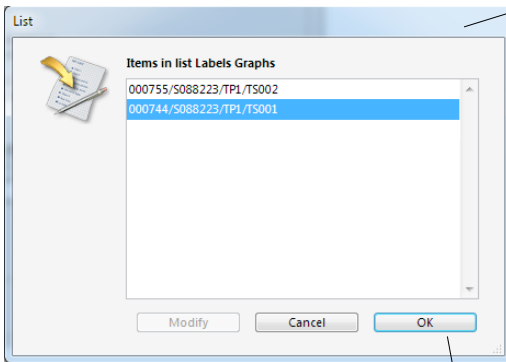

Choosing to search by User Reference, or Data Range will show all the matching data events for that search. This can involve several Data Labels' data. Checking the List All box will show all the saved Graphs.

Choose from the list presented and click OK to proceed.

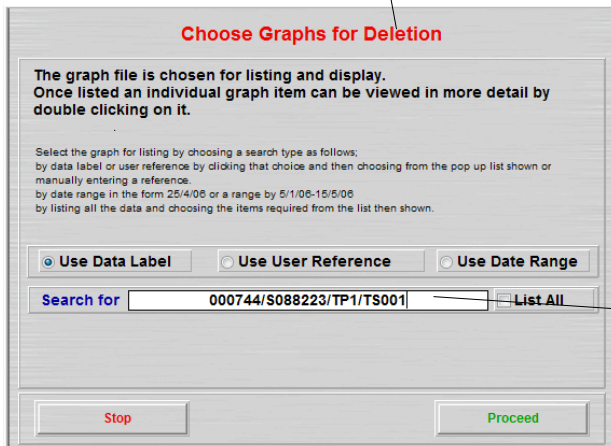

This Label is entered as the choice. Click confirm to proceed or click on the Search for entry point to choose again.

Listing of Graphs for Deletion

The stored graphs are then listed.

Graph Listing							
Select from the list below by clicking - shift clicking or control clicking. Reduce the selection to those required by clicking Reduce Selection. View Graphs by Double-clicking on the one required. Print the Graphs listed by clicking Print Selection.							
ID Graph	Data Label	User Reference	Start Date	Start Time	Finish Date	Finish Time	Origination
42	000744/S088223/TP1/TS001	SUR003	24/02/16	13:28:01	24/02/16	13:31:28	Created>25/02/2016
43	000744/S088223/TP1/TS001	SUR003	24/02/16	13:28:01	24/02/16	13:31:28	Created>25/02/2016
44	000744/S088223/TP1/TS001	SUR003	24/02/16	13:28:01	24/02/16	13:31:28	Created>25/02/2016
45	000744/S088223/TP1/TS001	SUR003	24/02/16	13:28:01	24/02/16	13:31:28	Created>25/02/2016
41	000744/S088223/TP1/TS001	SUR003	24/02/16	13:28:01	24/02/16	13:31:28	Created>25/02/2016


This completes this routine without deleting

This reduces the selection to only the graphs chosen. Highlight those required by clicking, shift clicking or control clicking

Double click to see the graph detail

These proceed to delete all the graphs listed above


You get one final chance to stop the deletion.

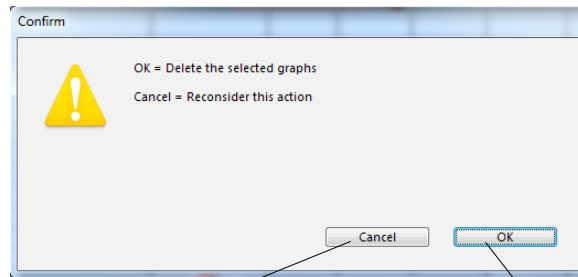

The graphs are not deleted



No more chances after this. The graphs are gone.

Delete Stored Certificates

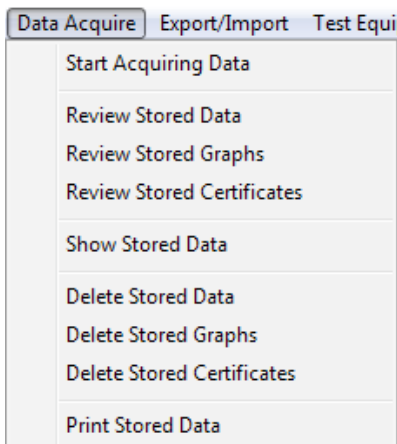


When this option is active this allows deleting of a created test certificate.

Print Stored Data

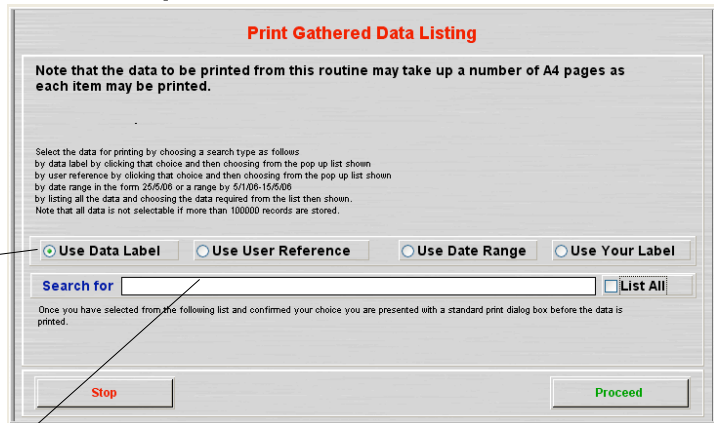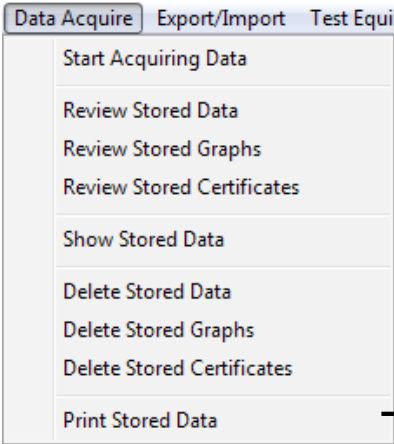

Choose the search type


Click on the search type or the Search for entry to show this pick list if you have chosen the Use Data Label

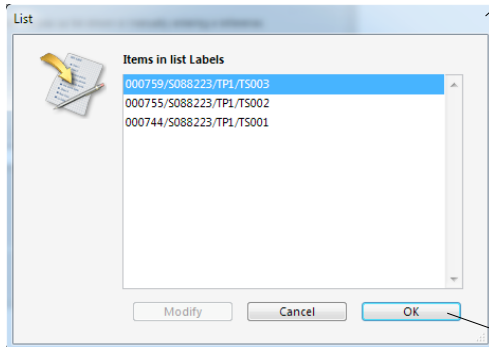

Click on the one required and then click OK to select this choice.

Choosing to search by User Reference, Data Range or Your Label will show all the matching data events for that search. This can involve several Data Labels' data. Checking the List All box will show all the stored data.

If the number of data items exceed the limit for displaying - default is 10,000 - then the data must be displayed either in blocks of 10,000 or by sampling the data to the limit of 10,000. The user is asked to choose which if this is the case.

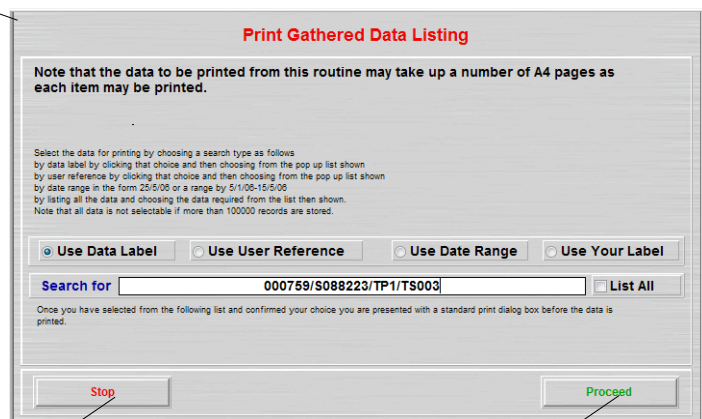

Click Stop to return to the start screen

Click Proceed to show the selected data

Listing of Data for Printing

The stored data items are then listed.

Data Acquired

Select from the list below by clicking, shift-clicking, control-clicking and then use Reduce Selection to leave just the records required on the list. Control-A selects all the data records. When the data is listed in blocks then Back and Next moves between blocks.

Data Label	User Reference	Data ID	Date	Time	Temp1	Temp2	Counters		
000759/S088223/TP1/TS003	SUR004	1565363	25/02/16	11:45:29	10.10	39.00 C	OFF Counts	OFF Counts	OFF Counts
Data 02/25/16	1: S080558ch1	230.1 barg	159.95 barg	484.6 barg	570 barg	404.4 barg	814.8 barg	994.8 barg	765.7 barg
000759/S088223/TP1/TS003	SUR004	1565364	25/02/16	11:45:30	10.10	39.00 C	OFF Counts	OFF Counts	OFF Counts
Data 02/25/16	2: S080558ch2	230.1 barg	159.94 barg	484.6 barg	570 barg	404.4 barg	814.8 barg	994.8 barg	765.7 barg
000759/S088223/TP1/TS003	SUR004	1565365	25/02/16	11:45:31	10.10	39.00 C	OFF Counts	OFF Counts	OFF Counts
Data 02/25/16	3: S080558ch3	230.1 barg	159.95 barg	484.6 barg	570 barg	404.4 barg	814.8 barg	994.8 barg	765.7 barg
000759/S088223/TP1/TS003	SUR004	1565366	25/02/16	11:45:32	10.10	39.00 C	OFF Counts	OFF Counts	OFF Counts
Data 02/25/16	4: S080558ch4	230.1 barg	159.94 barg	484.6 barg	570 barg	404.4 barg	814.8 barg	994.8 barg	765.7 barg
000759/S088223/TP1/TS003	SUR004	1565367	25/02/16	11:45:33	10.10	39.00 C	OFF Counts	OFF Counts	OFF Counts
Data 02/25/16	5: S080558ch5	230.3 barg	159.95 barg	484.6 barg	570 barg	404.4 barg	814.8 barg	994.8 barg	765.7 barg
000759/S088223/TP1/TS003	SUR004	1565376	25/02/16	11:45:42	1.20	22.00 C	OFF Counts	OFF Counts	OFF Counts
Data 02/25/16	6: S080558ch6	230.3 barg	159.95 barg	484.6 barg	570 barg	404.4 barg	814.8 barg	994.8 barg	765.7 barg
000759/S088223/TP1/TS003	SUR004	1565377	25/02/16	11:45:43	1.20	22.00 C	OFF Counts	OFF Counts	OFF Counts
Data 02/25/16	7: S080558ch7	230.3 barg	159.94 barg	484.6 barg	570 barg	404.4 barg	814.8 barg	994.8 barg	765.7 barg
000759/S088223/TP1/TS003	SUR004	1565378	25/02/16	11:45:44	1.90	21.90 C	OFF Counts	OFF Counts	OFF Counts
Data 02/25/16	8: S080558ch8	230.3 barg	159.94 barg	484.6 barg	570 barg	404.4 barg	814.8 barg	994.8 barg	765.7 barg

Finish
Restore All
Reduce Selection
Continue

This completes this routine

This returns the listing to the original list.


This reduces the selection to only those selected. Select by clicking - shift clicking or control clicking

If the data has been segmented to display in 10,000 blocks then next and back buttons appear to allow moving between blocks


This proceeds with this selection to printing

Double clicking on a listed item shows more detail.


If print to pdf is active then the data print pdfs are sent to the Save Location and the print screens do not appear

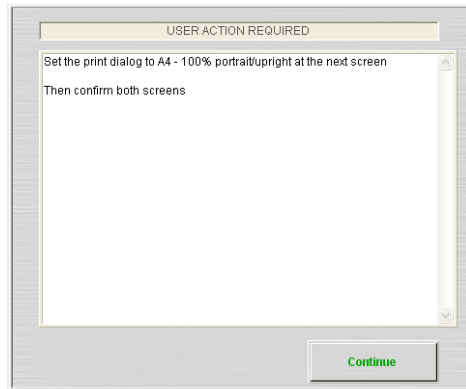

An information screen then appears advising the paper size as A4 and orientation as portrait or upright for the next screens

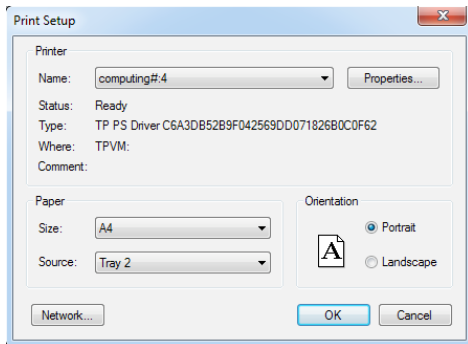

Set the values on the print settings screens and confirm both. Names and settings may vary for different printers

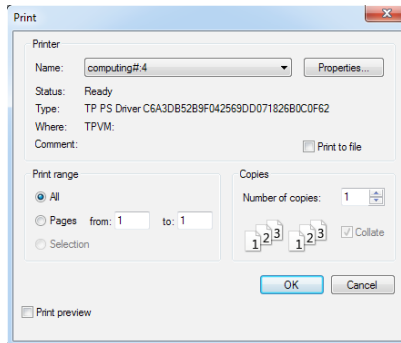

The print format is similar to this. Note that printing out the data may use a lot of paper.


Acquired Data Listing

Data Label				Date	Time	ID	Temperature
000828/S080560/TP1/TS003				14/03/2011	11:04:01	461118	10.40 13.70 C
Data 14/03/2011	SUR003			1 / 5	2 / 6	5 / 7	4 / 8
Counters 1 2 3	1:S080558ch1			0 barg	0 barg	0 barg	0 barg
-1	Counts	-1	Counts	-1	Counts	0 barg	0 barg
000828/S080560/TP1/TS003				14/03/2011	11:04:05	461119	10.40 13.70 C
Data 14/03/2011	SUR003			1 / 5	2 / 6	5 / 7	4 / 8
Counters 1 2 3	2:S080558ch2			0.01 barg	0 barg	0 barg	0 barg
-1	Counts	-1	Counts	-1	Counts	0 barg	0 barg
000828/S080560/TP1/TS003				14/03/2011	11:04:08	461120	10.40 13.70 C
Data 14/03/2011	SUR003			1 / 5	2 / 6	5 / 7	4 / 8
Counters 1 2 3	3:S080558ch3			100.08 barg	203.39 barg	143 barg	83 barg
-1	Counts	-1	Counts	-1	Counts	99.2 barg	99.2 barg
000828/S080560/TP1/TS003				14/03/2011	11:04:11	461121	10.40 13.70 C
Data 14/03/2011	SUR003			1 / 5	2 / 6	5 / 7	4 / 8
Counters 1 2 3	4:S080558ch4			210.83 barg	512.92 barg	393.9 barg	83 barg
-1	Counts	-1	Counts	-1	Counts	99.2 barg	99.2 barg
000828/S080560/TP1/TS003				14/03/2011	11:04:14	461122	10.40 13.70 C
Data 14/03/2011	SUR003			1 / 5	2 / 6	5 / 7	4 / 8
Counters 1 2 3	5:S080558ch5			210.83 barg	512.91 barg	393.9 barg	83 barg
-1	Counts	-1	Counts	-1	Counts	99.2 barg	99.2 barg
000828/S080560/TP1/TS003				14/03/2011	11:04:17	461123	10.30 13.80 C
Data 14/03/2011	SUR003			1 / 5	2 / 6	5 / 7	4 / 8
Counters 1 2 3	6:S080558ch6			210.83 barg	512.94 barg	393.9 barg	83 barg
-1	Counts	-1	Counts	-1	Counts	99.2 barg	99.2 barg
000828/S080560/TP1/TS003				14/03/2011	11:04:20	461124	10.40 13.70 C
Data 14/03/2011	SUR003			1 / 5	2 / 6	5 / 7	4 / 8
Counters 1 2 3	7:S080558ch7			210.83 barg	512.95 barg	393.9 barg	83 barg
-1	Counts	-1	Counts	-1	Counts	99.2 barg	99.2 barg
000828/S080560/TP1/TS003				14/03/2011	11:04:23	461125	10.40 13.70 C
Data 14/03/2011	SUR003			1 / 5	2 / 6	5 / 7	4 / 8
Counters 1 2 3	8:S080558ch8			210.83 barg	512.96 barg	393.9 barg	83 barg
-1	Counts	-1	Counts	-1	Counts	99.2 barg	99.2 barg
000828/S080560/TP1/TS003				14/03/2011	11:04:26	461126	10.40 13.70 C
Data 14/03/2011	SUR003			1 / 5	2 / 6	5 / 7	4 / 8
Counters 1 2 3	1:S080558ch1			210.83 barg	512.95 barg	393.9 barg	83 barg
-1	Counts	-1	Counts	-1	Counts	99.2 barg	99.2 barg
000828/S080560/TP1/TS003				14/03/2011	11:04:29	461127	10.30 13.70 C
Data 14/03/2011	SUR003			1 / 5	2 / 6	5 / 7	4 / 8
Counters 1 2 3	2:S080558ch2			210.83 barg	512.95 barg	393.9 barg	83 barg
-1	Counts	-1	Counts	-1	Counts	99.2 barg	99.2 barg
000828/S080560/TP1/TS003				14/03/2011	11:04:32	461128	10.40 13.70 C
Data 14/03/2011	SUR003			1 / 5	2 / 6	5 / 7	4 / 8
Counters 1 2 3	3:S080558ch3			210.83 barg	512.92 barg	393.9 barg	83 barg
-1	Counts	-1	Counts	-1	Counts	99.2 barg	99.2 barg

Export/Import Menu

Export Secure Data File

The data is saved using the search criterion as a label.

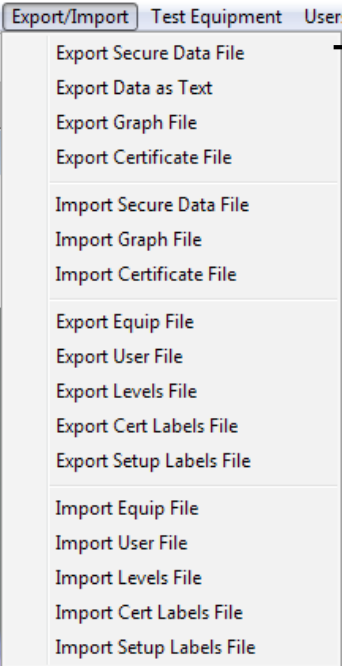

The data file exported by this routine is in a form that can only be read by the Import Secure Data File routine and cannot be viewed or changed by other programs. For the export of a normal text tab delineated file use 'Export Data as Text' menu item.



Choose the search type



Click Stop to return to the start screen

Click Proceed to show the selected data

If the number of data items exceed the limit for displaying - default is 10,000 - then the data must be displayed either in blocks of 10,000 or by sampling the data to the limit of 10,000. The user is asked to choose which if this is the case. The limit is for display ONLY. All of the data will be exported.

All the data that matches the search will be listed. When saved it will be labelled with the name in the Search for box

If the number of data items exceed the limit for displaying - default is 10,000 - then the data must be displayed either in blocks of 10,000 or by sampling the data to the limit of 10,000. The user is asked to choose which if this is the case. The limit is for display ONLY. All of the data that matches the search will be exported.

The stored data items are then listed.

Data Acquired

Select from the list below by clicking, shift-clicking, control-clicking and then use Reduce Selection to leave just the records required on the list. Control-A selects all the data records. When the data is listed in blocks then Back and Next moves between blocks.

Data Label	User Reference	Data ID	Date	Time	Temp1	Temp2	Counters		
000877/S088223/ZTP/test1	543	1577532	01/07/16	12:56:33	19.20	28.20 C	OFF Counts	OFF Counts	OFF Counts
Imported 07/07/16 1:S080558ch1	317.82 barg	0.3 barg	0.4 barg	1.4 barg	0Off	0Off	0Off	0Off	0Off
000877/S088223/ZTP/test1	543	1577533	01/07/16	12:56:36	19.20	28.20 C	OFF Counts	OFF Counts	OFF Counts
Imported 07/07/16 2:S080558ch2	317.84 barg	0.3 barg	0.4 barg	1.4 barg	0Off	0Off	0Off	0Off	0Off
000877/S088223/ZTP/test1	543	1577534	01/07/16	12:56:39	19.20	28.10 C	OFF Counts	OFF Counts	OFF Counts
Imported 07/07/16 3:S080558ch3	317.81 barg	0.29 barg	0.4 barg	1.4 barg	0Off	0Off	0Off	0Off	0Off
000877/S088223/ZTP/test1	543	1577535	01/07/16	12:56:42	19.20	28.10 C	OFF Counts	OFF Counts	OFF Counts
Imported 07/07/16 4:S080558ch4	317.81 barg	0.29 barg	0.4 barg	1.4 barg	0Off	0Off	0Off	0Off	0Off
000877/S088223/ZTP/test1	543	1577544	01/07/16	12:57:09	19.20	28.10 C	OFF Counts	OFF Counts	OFF Counts
Imported 07/07/16 5:	317.82 barg	0.29 barg	0.4 barg	1.4 barg	0Off	0Off	0Off	0Off	0Off

These sort the column above them up or down


This exits this routine without export

This returns the listing to the original list.

This reduces the selection to only those selected. Select by clicking - shift clicking or control clicking

If the data has been segmented to display in 10,000 blocks then next and back buttons appear to allow moving between blocks

This proceeds with this selection to export

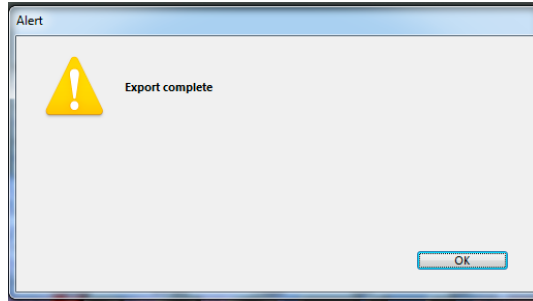



The data is exported in Secure Format to the assigned saving location. If the path is not found then you can choose to reset the path or save to the local export folder.

This screen confirms that the save has been successful

Export Data as Text

Note that it is important that you label the saved data in a way that avoids confusing the files.


The data file exported by this routine is in a form that can only be read into spreadsheets or word processors. It cannot be read into SDAS Review software from its text format. Use Export Secure Data File routine for that purpose.

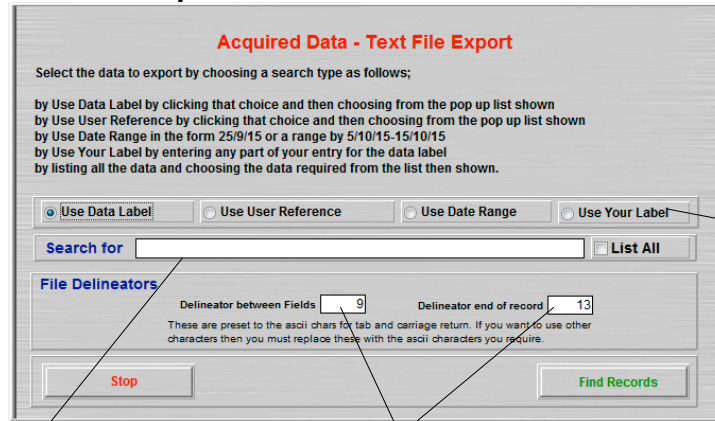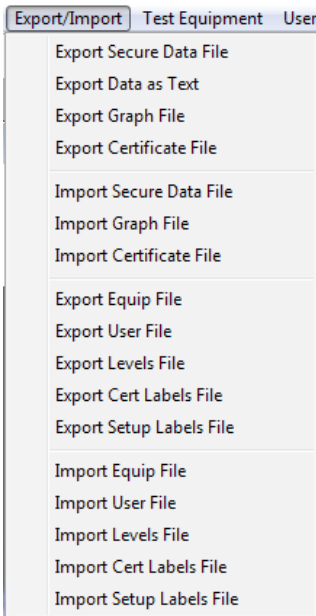

Choose the search type

Click on the search type or the Search for entry to show this pick list if you have chosen the Use Data Label


These allow the user to alter the value of the data delineators - the characters that appear between items and at the end of each record

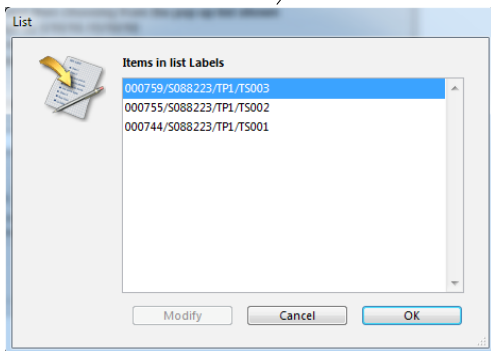

Choosing to search by User Reference, Data Range or Your Label will show all the matching data events for that search. This can involve several Data Labels' data. Checking the List All box will show all the stored data.


If the number of data items exceed the limit for displaying - default is 10,000 - then the data must be displayed either in blocks of 10,000 or by sampling the data to the limit of 10,000. The user is asked to choose which if this is the case. The limit is for display ONLY. All of the data will be exported.

Click on the one required and then click OK to select this choice.

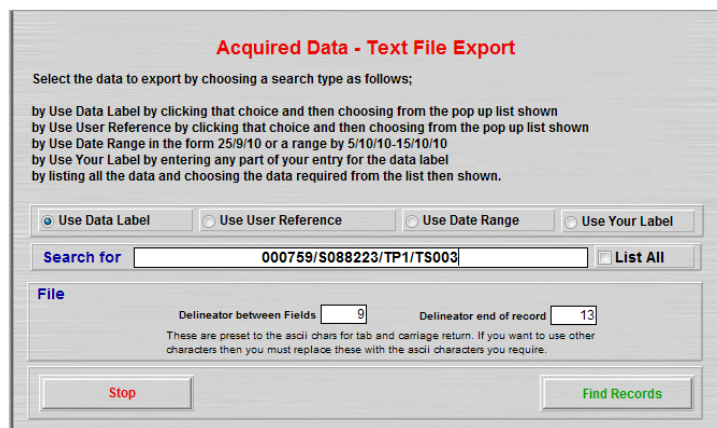



The rest of this routine is the same as Export Secure Data File

Export Graph File

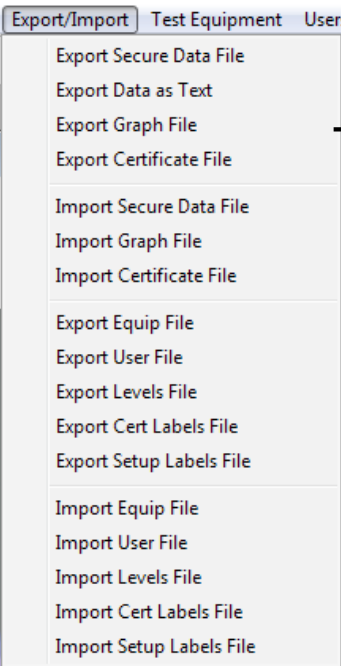


Note that it is important that you label the saved data in a way that avoids confusing the files.

The graph data file exported by this routine is in a form that can only be read by the SDAS Import Graph File routine and cannot be viewed or changed by other programs. The graph file cannot be exported as text.

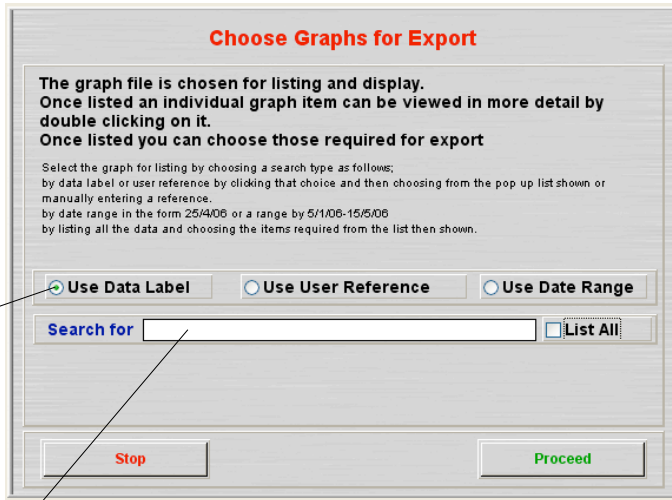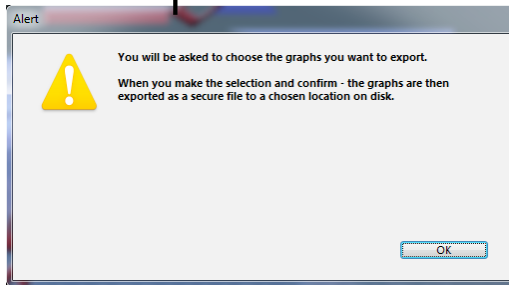


Choose the search type

Click on the search type or the Search for entry to show this pick list if you have chosen the Use Data Label

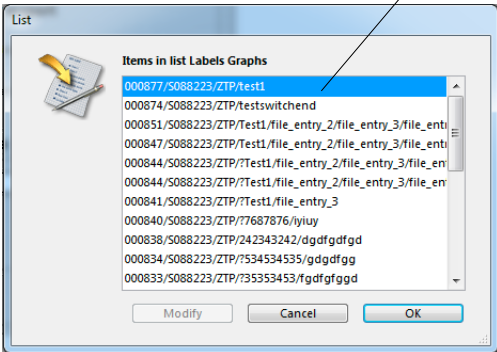

Choosing to search by User Reference, Data Range or Your Label will show all the matching data events for that search. This can involve several Data Labels' data. Checking the List All box will show all the stored graphs.

Click on the one required and then click OK to select this choice.

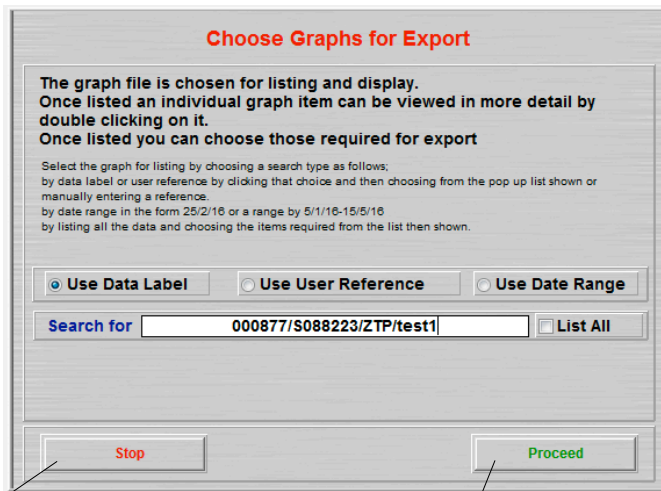

Click Stop to return to the start screen

Click Proceed to show the selected data


Stored Graph Listing

The stored graphs are then listed. The graphs are listed whether there is one found or many.

Graph Listing

Select from the list below by clicking - shift clicking or control clicking. Reduce the selection to those required by clicking Reduce Selection.
View Graphs by Double-clicking on the one required. Print the Graphs listed by clicking Print Selection.

ID Graph	Data Label	User Reference	Start Date	Start Time	Finish Date	Finish Time	Origination
78	000877/S088223/ZTP/test1	543	01/07/16	12:56:33	01/07/16	12:57:09	Created>08/07/2016
79	000877/S088223/ZTP/test1	543	01/07/16	12:56:33	01/07/16	12:57:09	Created>08/07/2016
80	000877/S088223/ZTP/test1	543	01/07/16	12:56:33	01/07/16	12:57:09	Created>08/07/2016
81	000877/S088223/ZTP/test1	543	01/07/16	12:56:33	01/07/16	12:57:09	Created>08/07/2016
82	000877/S088223/ZTP/test1	543	01/07/16	12:56:33	01/07/16	12:57:09	Created>08/07/2016
83	000877/S088223/ZTP/test1	543	01/07/16	12:56:33	01/07/16	12:57:09	Created>08/07/2016
84	000877/S088223/ZTP/test1	543	01/07/16	12:56:33	01/07/16	12:57:09	Created>08/07/2016
85	000877/S088223/ZTP/test1	543	01/07/16	12:56:33	01/07/16	12:57:09	Created>08/07/2016



These sort the column above them up or down


This completes this routine

This reduces the selection to only the graphs chosen. Highlight those required by clicking, shift clicking or control clicking


Continue to export data

The routine will export all the graphs listed above after showing the export data screens. Note that all the listed graphs will be saved if you do not select the one or ones required and then click Reduce Selection. You need to reduce the listed selection to ONLY the graphs you wish to export.


This screen appears to indicate that export has completed

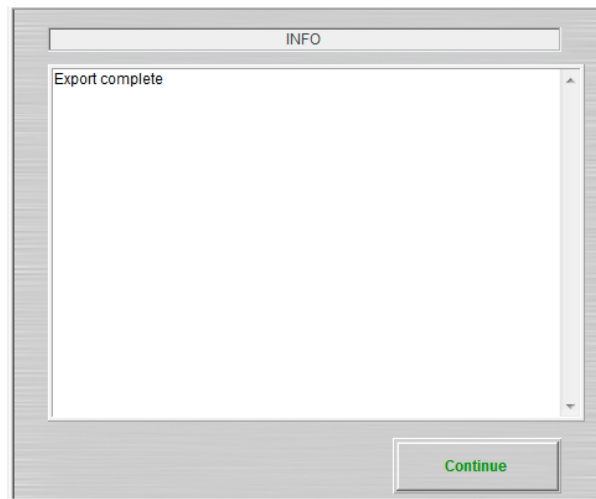


Export Certificates File

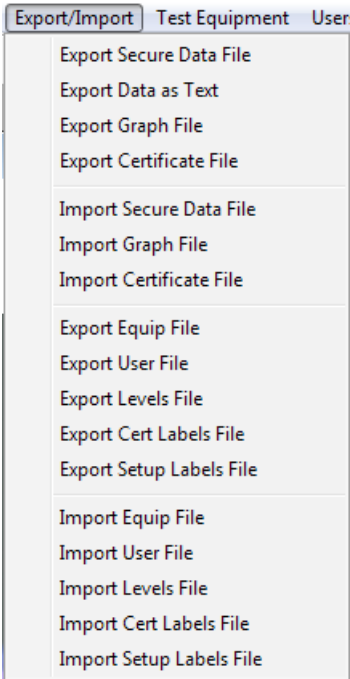

This option allows the export of certificate saved in the database to the normal save location. If this is not enabled then this alert screen appears.

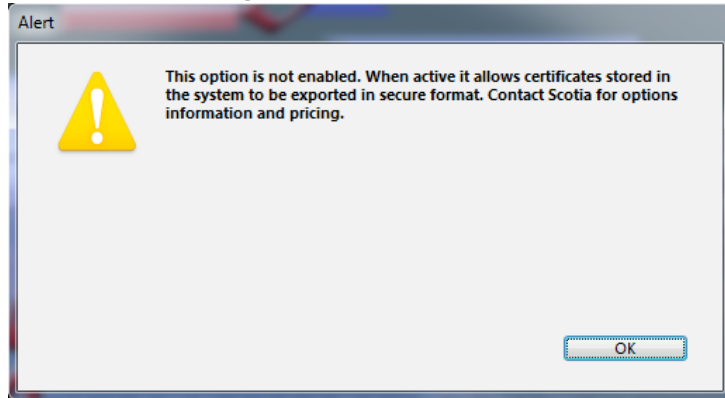


Import Secure Data File

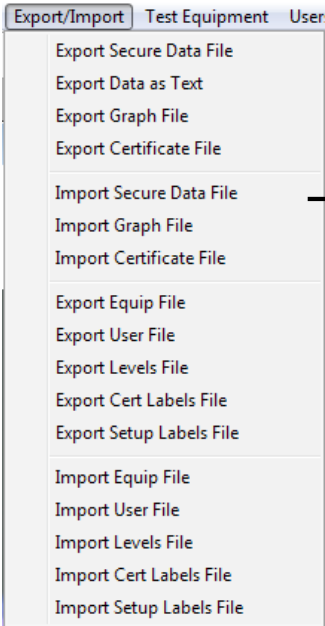


The data file imported by this routine is in a form that can only be read by the Import Secure Data File routine. Imported data is labelled as 'Imported' followed by the import date to distinguish it from gathered data.

If no files with the prefix ESD- are in the loading folder a screen appears to say that

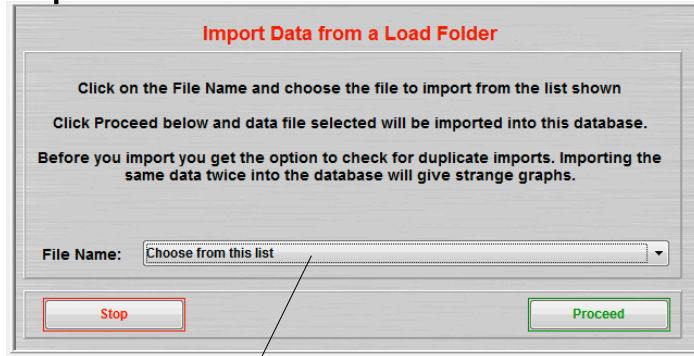


Click and choose from the pop up list of files available in the load folder

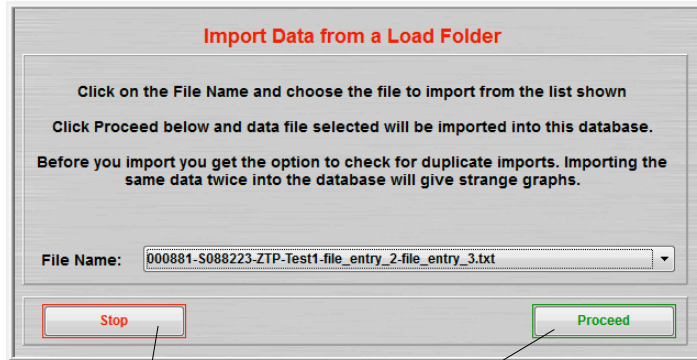

Click Stop aborts the import routine

Click Proceed to continue to load the file



It is possible to import the same file twice either entirely or partly. The system checks the type of file at import and if the file is not marked as a data file then importing is terminated. You can select to check for duplicates or not at import. If checking is on then any duplicates will be advised and the user is asked to decide to import or not. It may be that you know you have overlapped your export data by a few records so this routine will allow you to skip these and continue when the data is not being duplicated.

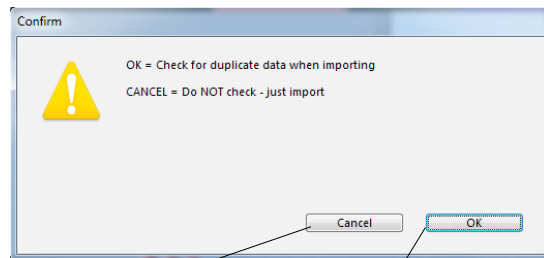

Click Cancel to import without checking

Click OK to check for duplicates on import


After the import the data choice lists need to be updated to reflect the new data in the files. In large databases this may take some time to rebuild so the option is given to delay this if you have other imports to do. You must do this at the end however otherwise the imported data will not appear in the pick lists.

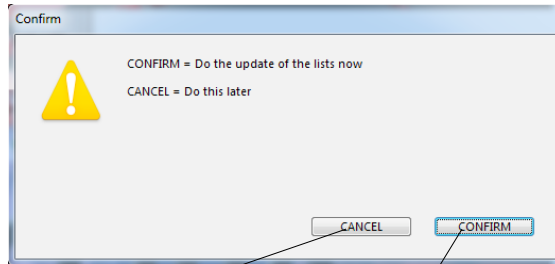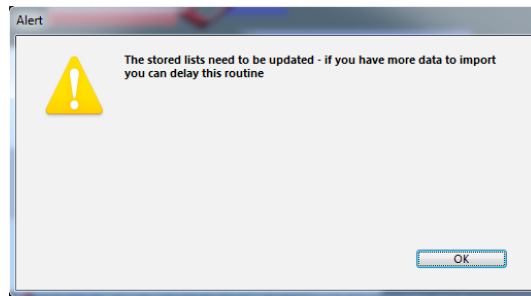


Click CANCEL to skip this just now

Click CONFIRM to proceed to do the list

If the import is successful then this screen appears to indicate that import has completed

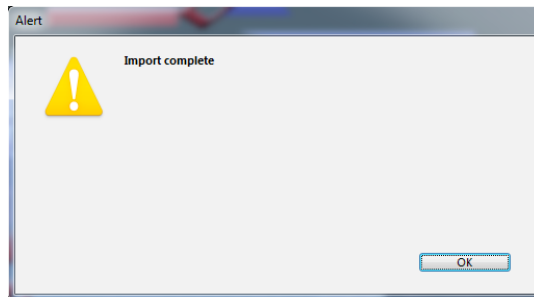


Import Graph File

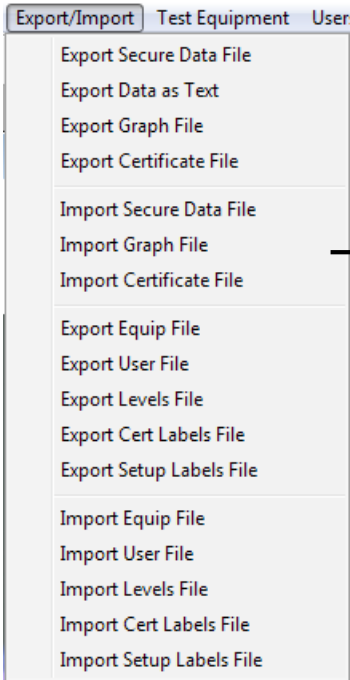


The graph data file imported by this routine is in a form that can only be read by the Import Graph File routine. Imported files are marked as Imported with the import date.

If no files with the prefix Gr- are in the loading folder a screen appears to say that

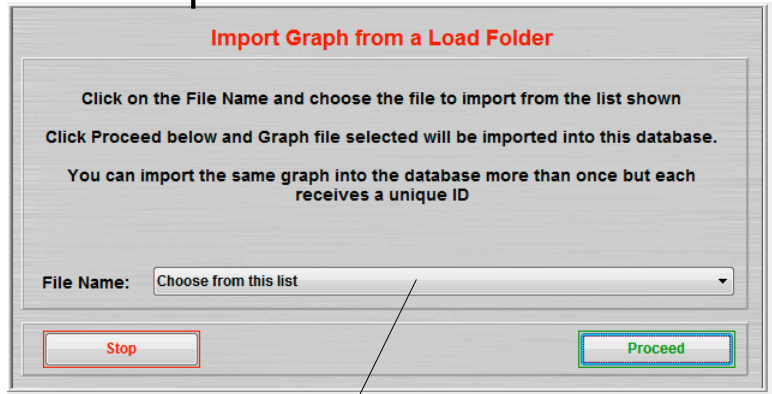


Click and choose from the pop up list of files available in the load folder

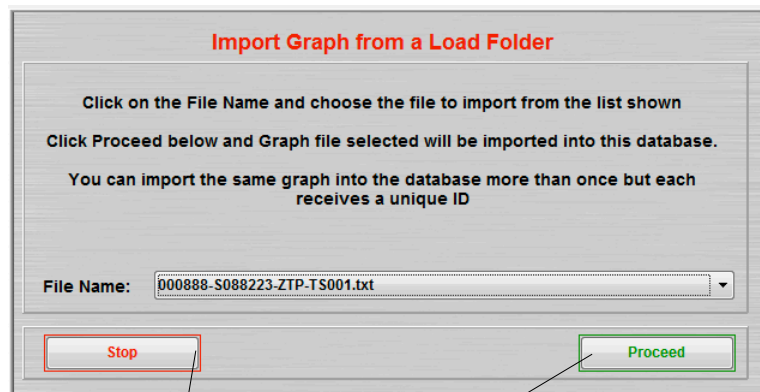


Click Stop aborts the import routine

Click Proceed to continue to load the file

This screen appears to indicate that import has completed

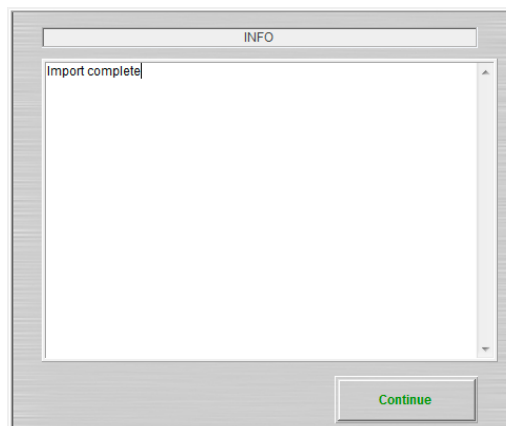


Import Certificates File

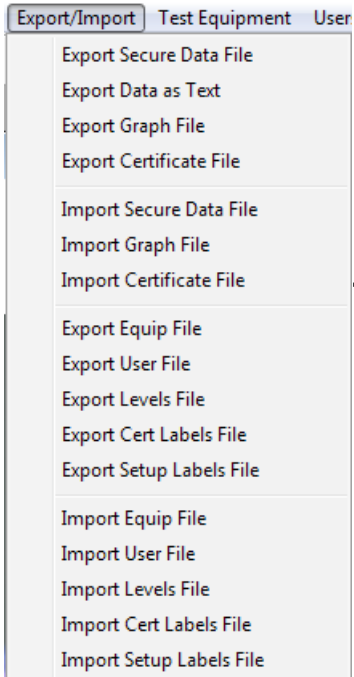


The certificate file imported by this routine is in a form that can only be read by the Import Certificate File routine. Imported files are marked as Imported with the import date.

If no files with the prefix C- are in the loading folder a screen appears to say that

If the certificates option is not enabled then this screen appears

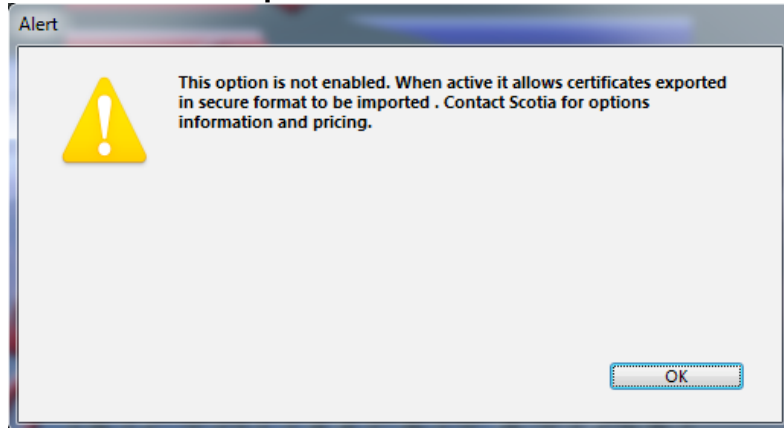


Export Equip File

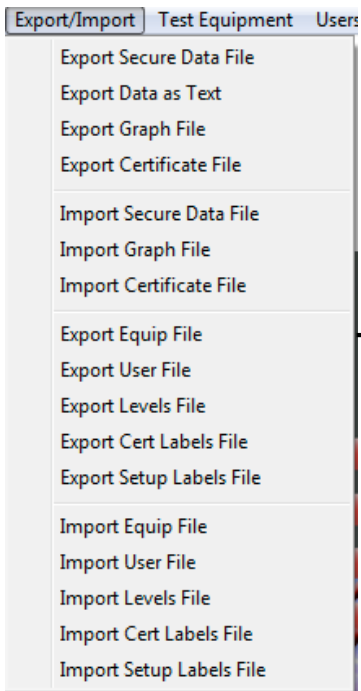


This allows the Equipment file from an SDAS to be exported in a form that can be read by another SDAS

The equipment file is exported to the save folder in the form EF-serial number-reverse date. The save folder is set in the Settings menu.

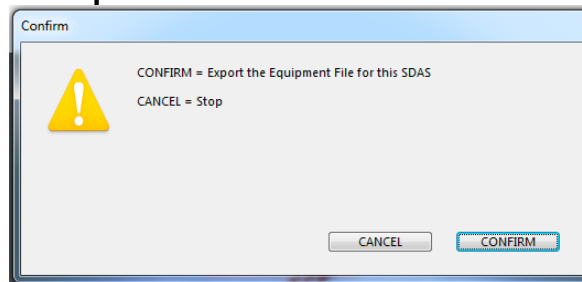


A confirmation of the export is given at the end of this routine.

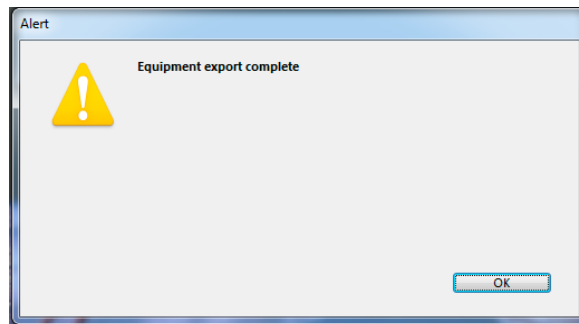

Export User File


Export Levels File

Export Cert Labels File

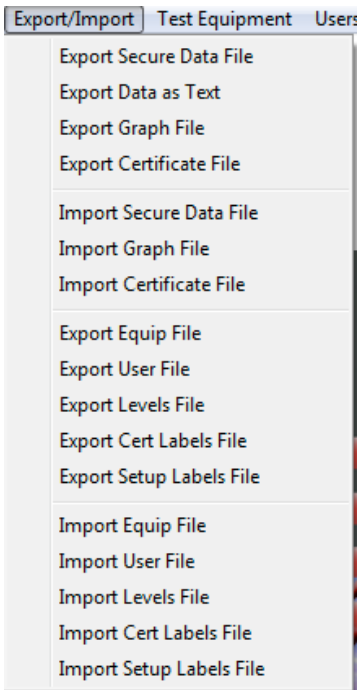


These are repeats of the Equipment file export above except they export the User File or Levels file or Certificate Labels file

Export Setup Labels File

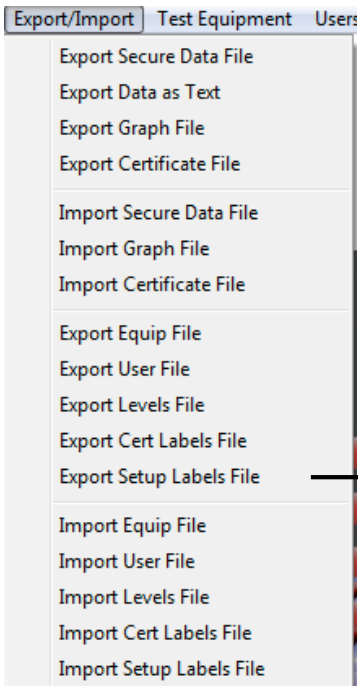

If the Enhanced Data option is enabled then this is a repeat of the Equipment file export above except it exports the Enhanced Data Labels File


Import Equip File

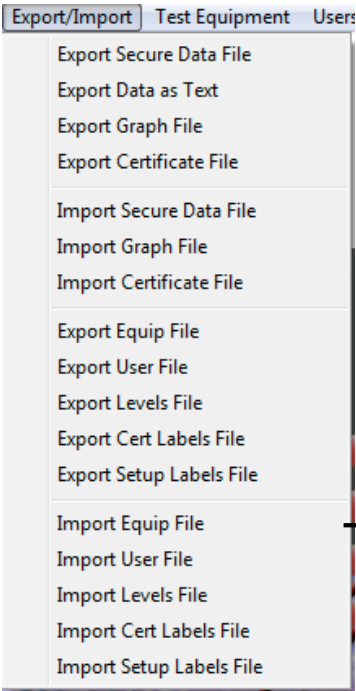


The equipment data file imported by this routine is in a form that can only be read by the Import Equipment File routine.

Files to be loaded must be in the Loading folder. This folder can be local, on a USB stick attached or a network location. The location must be set in the Settings menu.

If no files with the prefix EF- are in the loading folder a screen appears to say that

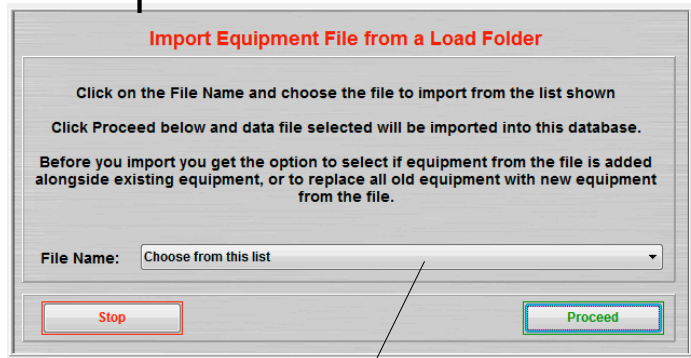


Click and choose from the pop up list of files available in the load folder

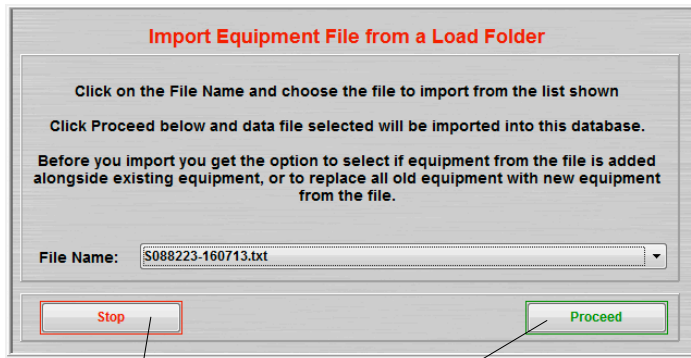

Click Stop aborts the import routine


Click Proceed to continue to load the file

The Equipment file can be added to the existing one or used to replace the existing one. Check the method you require.

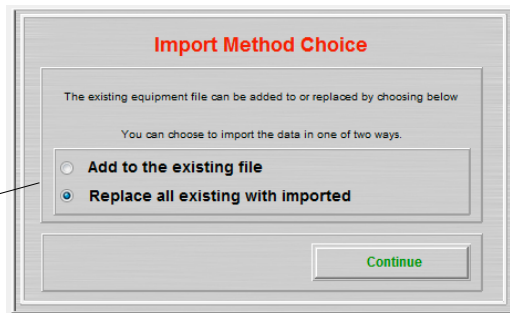

A check is applied to the file to ensure that you are importing a valid Equipment file. If the wrong header label is present then an alert appears and import stops


Since the Equipment file export is not selective - you must export all of the file - then you would only choose to add to the existing file if the transmitters etc on the exporting SDAS were additional to those currently on this SDAS. If you choose to add to the existing file then a duplicate check is applied to the data as it is imported. If any items with a matching chip ID or serial number are found the item will not be imported.

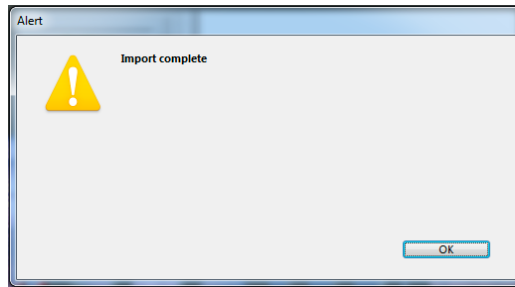

This screen appears to indicate that import has completed

Import User File


Import Level File

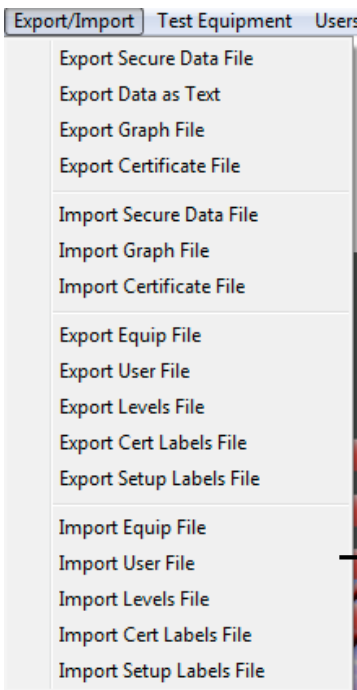

This is a repeat of the Equipment file import above except it imports the User File or Levels file. Note that the imported Levels file overwrites the current one.

Import Cert Labels File

Import Setup Labels File

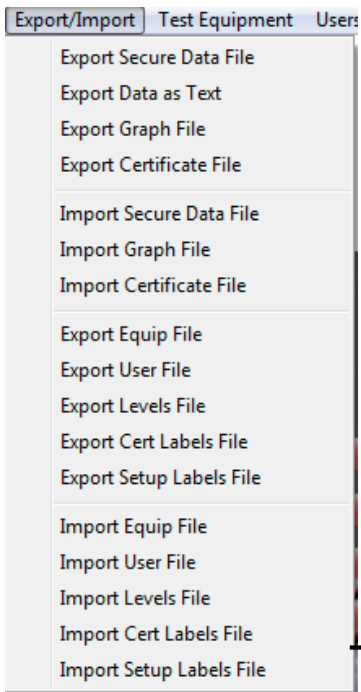

If the Certificates option is enabled then this is a repeat of the Equipment file import above except it imports the Certificate Labels File. Note that the imported Certificate Labels file overwrites the current one.

If the Enhanced Data option is enabled then this is a repeat of the Equipment file import above except it imports the Enhanced Data Labels File. Note that the imported Enhanced Data Labels file overwrites the current one.

Test Equipment Menu

All transmitters used must be registered in the Equipment file. In Server based systems the SDAS device must also be registered in this file.

List Equipment

Test Equipment Users Demo Utilities

- List Equipment
- Create Equipment
- Amend Equipment
- Cal of A to D
- Get Connected Chip IDs
- Get Connected Transmitters

This allows items of equipment in the database system to be viewed.

Stored Equipment Listing

Equip ID	Description	Type	Status	Ser No	Chip No	Range from	Range to	Units
1	SUDS	ScotiaLogger3	Current	SDL1	EFC1BA4	0	10	bar
2	Channel 1	Transmitter	Current	2643815	EFC50E7	-1000	0	mbarg
3	Channel 2	Transmitter	Current	2643813	E9013BD	0	689	bar
4	Channel 3	Transmitter	Current	2643812	EFC27E3	0	1100	bar
5	Channel 4	Transmitter	Current	2643814	EFC2A8	0	400	bar
6	Channel 5	Transmitter	Current	2643810	EFB22B	0	250	bar
7	Trans	Transmitter	Current	123456	11DE0440	0	689	bar
8	Trans	Transmitter	Current	123457	10A0B34	0	100	bar
9	Trans	Transmitter	Current	123458	10FC1D62	0	200	bar
10	Temp Probe	Temp Probe 1	Current	S080575T1	S080575T1	0	100	deg C
11	Scotialogger 4	ScotiaLogger3	Current	S080575	11DE8AF5	0	100	bar
12	Ambient Temp	Temp Probe 2	Current	S080575T2	S080575T2	0	100	deg C
13	SIM_CH5	Transmitter	Current	805745	11031EA	0	100	MPa
14	SIM_CH4	Transmitter	Current	805744	10FFEB94	0	250	bar
15	SIM_CH3	Transmitter	Current	805743	10FF3A1	0	1600	mbar
16	SIM_CH2	Transmitter	Current	805742	110323	0	10000	psi
17	SIM_CH1	Transmitter	Current	805741x	11051A9	0	700	bar
18	MarkPlug	Transmitter	Current	MarkPlug	15A13319	0	1000	bar
19	Tx	Transmitter	Current	A123	A473AF1	0	1000	psi
20	Tx	Transmitter	Current	A124	A48F20	0	2000	psi
21	Tx	Transmitter	Current	A125	A475C43	0	4000	psi
22	Tx	Transmitter	Current	A126	A563AD1	0	5000	psi
23	Tx	Transmitter	Current	A127	A481BF1	0	7500	psi
24	Tx	Transmitter	Current	A129	A45E2F3	0	10000	psi
25	Tx	Transmitter	Current	A128	A467EF2	0	30000	psi
26	Tx	Transmitter	Current	A130	A462EE1	0	15000	psi
27	Channel 1	Transmitter	Current	2643815	9E0571A	0	1000	bar
28	Channel 2	Transmitter	Current	2643813	9DFE7E3	0	700	bar

Reduce Selection Continue

The list can be sorted ascending or descending by column by clicking the up or down arrow

The list can be reduced to those selected by clicking the Reduce Selection

This ends this routine

Double click on the item to be see more detail

Test Equipment


Enter the Equipment Details below

Device Serial Number	123457	Enter the equipment marked serial number. This is a unique field so enter something unique.
Description	Trans	Enter a meaningful description
Type	Transmitter	Choose from the list offered
Range from	0	Enter the range of the transmitters and
Range to	100	
Units	bar	Choose from the list or enter your own units
Calibration Date	00/00/00	Enter the calibration info on the device
Calibration Reference		
Recalibration Date	00/00/00	
Measuring Quantity	Pressure	Choose from the list offered or enter your own measuring quantity
Scotia Chip Serial No	10A0B34	Enter the chip ID for transmitters. This is a unique field so enter something unique.
Device Status	Current	Choose from the list offered

Stop Confirm

The items are labelled to indicate their meaning. The calibration detail can be used to store the calibration dates and traceable references for the equipment.

Create Equipment

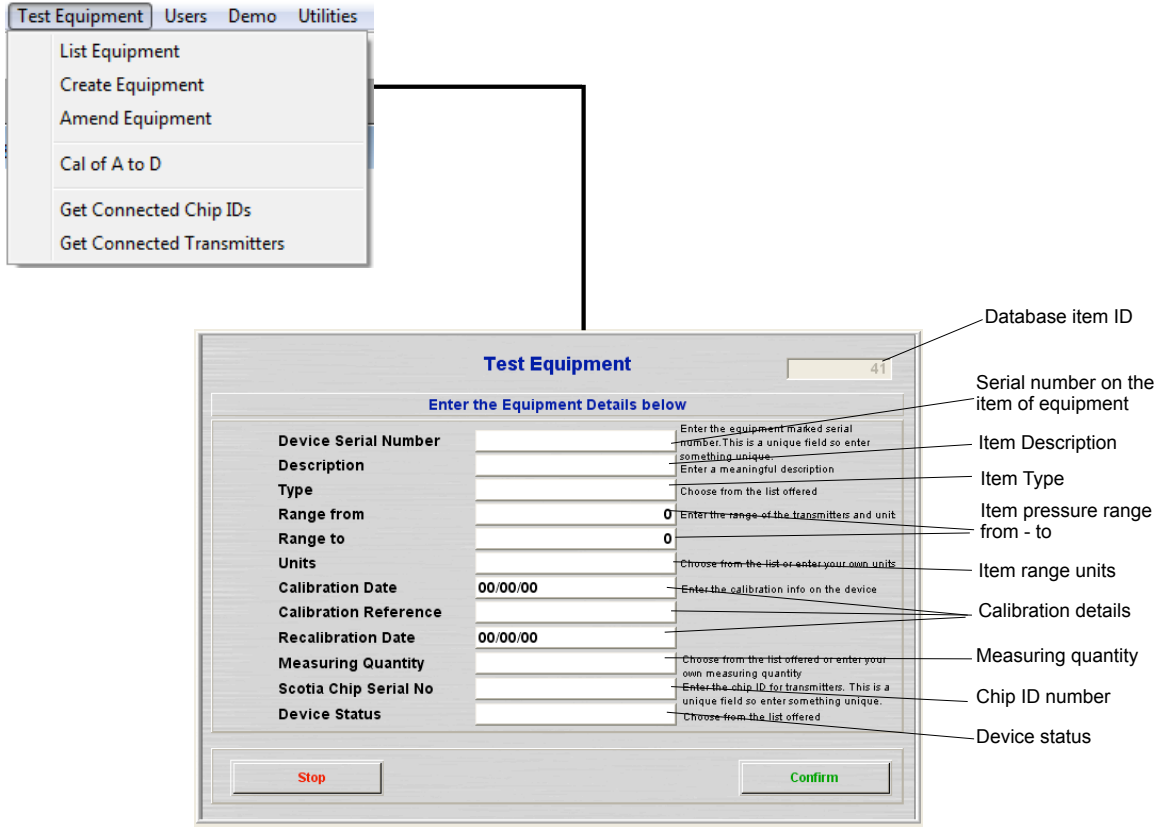

The serial number should be that marked on the transmitter. This entry is unique and any duplication will not be accepted.

The Description should be that of the transmitter - manufacturer, model etc.

Item type has to be chosen from the pop-up list that appears. Note: only items with type 'transmitter' will appear in the list of test equipment for choosing a transmitter.

Item pressure range. This MUST be the calibrated range of the transmitter. The SDAS unit will assume that when 4 mA is being read that the transmitter is at the lower value of the scale entered and that when 20 mA is being read that the transmitter is at full scale. Failure to comply with this will compromise the operation of the SDAS.

Units MUST be the units of the transmitter calibrated range.

Calibration Date, reference, and Recalibration date are optional. An additional option to the SDAS system can control this information warning the user of calibration becoming due etc.

Measuring quantity is the physical property being measured by the transmitter e.g. pressure. This can be chosen from the pop-up list or entered manually.

Chip ID number is the chip fitted to the transmitter. This must be correct for the transmitter to be used in the SDAS. Any detected chip that is not included in this file will not be accepted for use by the SDAS system until it has been entered in this file.

If no chip has been fitted to the transmitter then enter the item serial number. Do not leave this entry blank. This entry is unique and any duplication will not be accepted.

Device status is the current status of the transmitter. Only 'current' items will be included in any pop-up list.

Filled with sample data

Test Equipment 42

Enter the Equipment Details below

Device Serial Number	654321	Enter the equipment marked serial number. This is a unique field so enter something unique.
Description	Channel 1	Enter a meaningful description.
Type	Transmitter	Choose from the list offered.
Range from	0	Enter the range of the transmitters and
Range to	1000	
Units	barg	Choose from the list or enter your own units.
Calibration Date	00/00/00	Enter the calibration info on the device.
Calibration Reference		
Recalibration Date	00/00/00	
Measuring Quantity	Pressure	Choose from the list offered or enter your own measuring quantity.
Scotia Chip Serial No	9E0571B	Enter the chip ID for transmitters. This is a unique field so enter something unique.
Device Status	Current	Choose from the list offered.

If the calibration check option is active then calibration and recalibration dates are checked when entered

Do not add this item

Add this item to the database and pop-up lists

Amend Equipment

Test Equipment Users Demo Utilities

- List Equipment
- Create Equipment
- Amend Equipment
- Cal of A to D
- Get Connected Chip IDs
- Get Connected Transmitters

This allows items of equipment to be amended in the database system. These amendments then update the transmitter pick list used when starting a test.

Stored Equipment Listing

Equip ID	Description	Type	Status	Ser No	Chip No	Range from	Range to	Units
11	Scotialogger 4	ScotiaLogger3	Current	S080575	11DE8AF5	0	100	barg
12	Ambient Temp	Temp Probe 2	Current	S080575T2	S080575T2	0	100	deg C
13	SIM_CH5	Transmitter	Current	805745	11031EA	0	100	MPa
14	SIM_CH4	Transmitter	Current	805744	10FFEB94	0	250	barg
15	SIM_CH3	Transmitter	Current	805743	10FFF3A1	0	1600	mbar
16	SIM_CH2	Transmitter	Current	805742	110323	0	10000	psi
17	SIM_CH1	Transmitter	Current	805741x	11051A9	0	700	barg
18	MarkPlug	Transmitter	Current	MarkPlug	15A13319	0	1000	barg
19	Tx	Transmitter	Current	A123	A473AF1	0	1000	psi
20	Tx	Transmitter	Current	A124	A46F20	0	2000	psi
21	Tx	Transmitter	Current	A125	A475C43	0	4000	psi
22	Tx	Transmitter	Current	A126	A563AD1	0	5000	psi
23	Tx	Transmitter	Current	A127	A481BF1	0	7500	psi
24	Tx	Transmitter	Current	A128	A45E2F3	0	10000	psi
25	Tx	Transmitter	Current	A128	A467EF2	0	30000	psi
26	Tx	Transmitter	Current	A130	A462EE1	0	15000	psi
27	Channel 1	Transmitter	Current	2643815	9E0571A	0	1000	barg
28	Channel 2	Transmitter	Current	2643813	9DFE7E3	0	700	barg
29	Channel 3	Transmitter	Current	2643812	9E06B	0	1100	barg
30	Channel 4	Transmitter	Current	2643814	9C7A08C	0	400	barg
31	Channel 5	Transmitter	Current	2643810	9E07736	0	250	barg
32	Test CH1	Transmitter	Current	S080558ch1	14798E11	0	1000	barg
33	Test CH2	Transmitter	Current	S080558ch2	14798B214	0	750	barg
34	Test CH3	Transmitter	Current	S080558ch3	147A89C0	0	1000	barg
35	Test CH4	Transmitter	Current	S080558ch4	1479A4F4	0	1000	barg
36	Test CH5	Transmitter	Current	S080558ch5	147941D	0	1250	barg
37	Test CH6	Transmitter	Current	S080558ch6	147834E4	0	1250	barg
38	Test CH7	Transmitter	Current	S080558ch7	147A8E15	0	1500	barg
39	Test CH8	Transmitter	Current	S080558ch8	147A8EC	0	1500	barg
40	Temp1	Temp Probe 1	Current	S080558T1	147A8DE2	0	100	deg C
41	Temp2	Temp Probe 2	Current	S080558T2	147A5FDD	0	100	deg C

Reduce Selection Continue

The list can be sorted ascending or descending by column by clicking the up or down arrow

Double click on the item to be see more detail

The list can be reduced to those selected by clicking the Reduce Selection

This ends this routine

Test Equipment 18

Enter the Equipment Details below

Device Serial Number	<input type="text" value="MarkPlug"/>	Enter the equipment marked serial number. This is a unique field so enter something unique.
Description	<input type="text" value="MarkPlug"/>	Enter a meaningful description
Type	<input type="text" value="Transmitter"/>	Choose from the list offered
Range from	<input type="text" value="0"/>	Enter the range of the transmitters and
Range to	<input type="text" value="1000"/>	
Units	<input type="text" value="barg"/>	Choose from the list or enter your own units
Calibration Date	<input type="text" value="00/00/00"/>	Enter the calibration info on the device
Calibration Reference	<input type="text"/>	
Recalibration Date	<input type="text" value="00/00/00"/>	
Measuring Quantity	<input type="text" value="Other"/>	Choose from the list offered or enter your own measuring quantity
Scotia Chip Serial No	<input type="text" value="15A13319"/>	Enter the chip ID for transmitters. This is a unique field so enter something unique.
Device Status	<input type="text" value="Current"/>	Choose from the list offered

Stop Confirm

This resets any changes made to this item

This confirms any changes

Cal of A to D

NOTE THAT CONFIRMING THAT YOU HAVE THE VALUE APPLIED IN THE FOLLOWING SCREENS WHEN YOU DO NOT WILL RENDER THE OPERATION OF THE SDAS INSTRUMENT INACCURATE UNTIL YOU DO THE CALIBRATION PROPERLY. IF A CALIBRATION FAILED MESSAGE IS GIVEN AT THE END THEN YOU SHOULD NOT USE THE SDAS UNTIL AN ACCEPTABLE CALIBRATION IS DONE. ACCESS TO THIS MENU ITEM SHOULD BE SEVERELY RESTRICTED.

The routine below shows the calibration routine for a 2016 model SDAS or ScotiaDatabox using 601 version software. The routine below is for the 8-channel model. If you have one with fewer channels then choose the routine that matches the number of channels fitted to the SDAS. You must calibrate all the channels fitted even if you use fewer than the full number available.

Note also that you must perform the calibration of both temperature inputs.

Be prepared to do this before you start this routine. Stopping the routine and aborting may result in a partial calibration.

This routine calibrates the A to D device that reads the current flowing in the transmitter and calibrates the component that measures the pt-100 probes output. Note: Like any instrument the calibration is vital to its correct operation so this routine should only be performed by a technician skilled at calibrating instruments and who is using traceable equipment capable of simulating a 4-20mA transmitter and a Pt-100 probe. Failure to calibrate correctly may render the SDAS inoperable.

Test Equipment Users Demo Utilities

- List Equipment
- Create Equipment
- Amend Equipment
- Cal of A to D
- Get Connected Chip IDs
- Get Connected Transmitters

SDAS Calibration Routine

To operate this routine requires that you have instrumentation that can provide a calibrated output of 4-20 mA and a Pt-100 simulation of 0-100 C

Calibration Notes

This routine provides a calibration routine for the various SDAS and ScotiaDatabox units. The correct routine for this model of SDAS or ScotiaDatabox should be selected from the choice of 2 routines below.

Note the following before you start this calibration routine:

Second Temperature calibration: The second temperature is calibrated in this routine even if this option is not active in this SDAS. You must apply the requested values to the input port for the second temperature when requested by the routine. Failure to do this will cause a failure of the calibration routine.

Counters: Calibration for counters is done with a known number of pulses being applied to the counter input. These are checked against the actual number counted in the normal acquisition routine and not in this calibration routine.

This calibration should be carried out by a trained technician. Failure to apply the correct values to the correct ports when requested may result in I/O board routines failing. The normal SDAS checks cannot be made during this operation as the calibration is performed on the I/O board routines directly. Be especially careful in applying the requested values to the ports at the right time.

Exit Cal routine Routine for SDAS with 1 channel Routine for SDAS with 5 channels Routine for SDAS with 8 channels

Exit Routine Single Channel SDAS 5 Channel SDAS 8 Channel SDAS

This exits the routine

This is the routine for the original single channel SDAS units. This was the original SDAS unit and is covered here for completeness.

This is the routine for SDAS units that have 5 x 4-20mA inputs. THE FOLLOWING ROUTINE SHOWS TO THIS SELECTION.

This is the routine for SDAS units that have 8 x 4-20mA inputs. This is same as the 5 channel except it continues for another 3 channels.

The 5 channel is illustrated here but the 8 channel routine just has different labeling and 3 more channels in the routine. The single channel SDAS stops after the temperature calibration.

This screen appears next

SDAS Calibration Routine

To operate this routine requires that you have instrumentation that can provide a calibrated output of 4-20 mA and a Pt-100 simulation of 0-100 C

Start of Calibration routine. Apply 4mA to the SDAS Channel 1 input

Apply this value to Channel 1 Input

4 mA

Confirm Value Set

End Routine

This routine sets the 4 and 20 mA of the 5 channels of the AtoD system. A full calibration check can be performed afterwards by either calibrating real transmitters on each of the ranges or using the 4-20mA calibration device as input in each the 5 channels, selecting the calibration item from the list of test equipment and applying as many points as you require across the scale of the transmitter or simulator.

The transmitters used with this device should be calibrated across their 4-20mA range. You should ensure that the calibration range is entered in the Test Equipment section of this database. These two calibrations will link to give the equivalent of a calibration of the whole system calibrated together. Alternatively the transmitter can be connected and calibrated with the SDAS by using the normal data acquisition routine.

Click this when you have 4 mA set on the mA input. Check this before you click.

If you wish to abort this routine click this. Note that calibration points up to this point will still be stored in the SDAS A/D system.

This screen appears next

SDAS Calibration Routine

To operate this routine requires that you have instrumentation that can provide a calibrated output of 4-20 mA and a Pt-100 simulation of 0-100 C

Apply 20mA to the SDAS Channel 1 input

Apply this value to Channel 1 Input

20 mA

Confirm Value Set

End Routine

This routine sets the 4 and 20 mA of the 5 channels of the AtoD system. A full calibration check can be performed afterwards by either calibrating real transmitters on each of the ranges or using the 4-20mA calibration device as input in each the 5 channels, selecting the calibration item from the list of test equipment and applying as many points as you require across the scale of the transmitter or simulator.

The transmitters used with this device should be calibrated across their 4-20mA range. You should ensure that the calibration range is entered in the Test Equipment section of this database. These two calibrations will link to give the equivalent of a calibration of the whole system calibrated together. Alternatively the transmitter can be connected and calibrated with the SDAS by using the normal data acquisition routine.

Click this when you have 20 mA set on the mA input. Check this before you click.

If you wish to abort this routine click this. Note that calibration points up to this point will still be stored in the SDAS A/D system.

This screen appears next

SDAS Calibration Routine

To operate this routine requires that you have instrumentation that can provide a calibrated output of 4-20 mA and a Pt-100 simulation of 0-100 C

Main Temp Probe Cal
Apply 0 degC as 100 Ohms to the SDAS Temperature 1 input

Apply this value to Temp 1

This routine sets the 4 and 20 mA of the 5 channels of the AtoD system. A full calibration check can be performed afterwards by either calibrating real transmitters on each of the ranges or using the 4-20mA calibration device as input in each the 5 channels, selecting the calibration item from the list of test equipment and applying as many points as you require across the scale of the transmitter or simulator.

The transmitters used with this device should be calibrated across their 4-20mA range. You should ensure that the calibration range is entered in the Test Equipment section of this database. These two calibrations will link to give the equivalent of a calibration of the whole system calibrated together. Alternatively the transmitter can be connected and calibrated with the SDAS by using the normal data acquisition routine.

Click this when you have 100 Ohms or 0 degC set on the Temperature 1 input. Check this before you click.

If you wish to abort this routine click this. Note that calibration points up to this point will still be stored in the SDAS A/D system.

This screen appears next

SDAS Calibration Routine

To operate this routine requires that you have instrumentation that can provide a calibrated output of 4-20 mA and a Pt-100 simulation of 0-100 C

Main Temp Probe Cal
Apply 100 degC as 138.5 Ohms to the SDAS Temperature 1 input

Apply this value to Temp 1

This routine sets the 4 and 20 mA of the 5 channels of the AtoD system. A full calibration check can be performed afterwards by either calibrating real transmitters on each of the ranges or using the 4-20mA calibration device as input in each the 5 channels, selecting the calibration item from the list of test equipment and applying as many points as you require across the scale of the transmitter or simulator.

The transmitters used with this device should be calibrated across their 4-20mA range. You should ensure that the calibration range is entered in the Test Equipment section of this database. These two calibrations will link to give the equivalent of a calibration of the whole system calibrated together. Alternatively the transmitter can be connected and calibrated with the SDAS by using the normal data acquisition routine.

Click this when you have 138.5 Ohms or 100 degC set on the Temperature 1 input. Check this before you click.

If you wish to abort this routine click this. Note that calibration points up to this point will still be stored in the SDAS A/D system.

This screen appears next

SDAS Calibration Routine

To operate this routine requires that you have instrumentation that can provide a calibrated output of 4-20 mA and a Pt-100 simulation of 0-100 C

Ambient Temp Probe Cal
Apply 0 degC as 100 Ohms to the SDAS Temperature 2 input

Apply this value to Temp 2

100 Ohms

Confirm Value Set

End Routine

This routine sets the 4 and 20 mA of the 5 channels of the AtoD system. A full calibration check can be performed afterwards by either calibrating real transmitters on each of the ranges or using the 4-20mA calibration device as input in each the 5 channels, selecting the calibration item from the list of test equipment and applying as many points as you require across the scale of the transmitter or simulator.

The transmitters used with this device should be calibrated across their 4-20mA range. You should ensure that the calibration range is entered in the Test Equipment section of this database. These two calibrations will link to give the equivalent of a calibration of the whole system calibrated together. Alternatively the transmitter can be connected and calibrated with the SDAS by using the normal data acquisition routine.

Click this when you have 100 Ohms or 0 degC set on the Temperature 2 input. Check this before you click.

If you wish to abort this routine click this. Note that calibration points up to this point will still be stored in the SDAS A/D system.

This screen appears next

SDAS Calibration Routine

To operate this routine requires that you have instrumentation that can provide a calibrated output of 4-20 mA and a Pt-100 simulation of 0-100 C

Ambient Temp Probe Cal
Apply 100 degC as 138.5 Ohms to the SDAS Temperature 2 input

Apply this value to Temp 2

138.5 Ohms

Confirm Value Set

End Routine


This routine sets the 4 and 20 mA of the 5 channels of the AtoD system. A full calibration check can be performed afterwards by either calibrating real transmitters on each of the ranges or using the 4-20mA calibration device as input in each the 5 channels, selecting the calibration item from the list of test equipment and applying as many points as you require across the scale of the transmitter or simulator.

The transmitters used with this device should be calibrated across their 4-20mA range. You should ensure that the calibration range is entered in the Test Equipment section of this database. These two calibrations will link to give the equivalent of a calibration of the whole system calibrated together. Alternatively the transmitter can be connected and calibrated with the SDAS by using the normal data acquisition routine.


Click this when you have 138.5 Ohms or 100 degC set on the Temperature 2 input. Check this before you click.

If you wish to abort this routine click this. Note that calibration points up to this point will still be stored in the SDAS A/D system.

The 4-20mA calibration screen appear for each channel now in sequence.

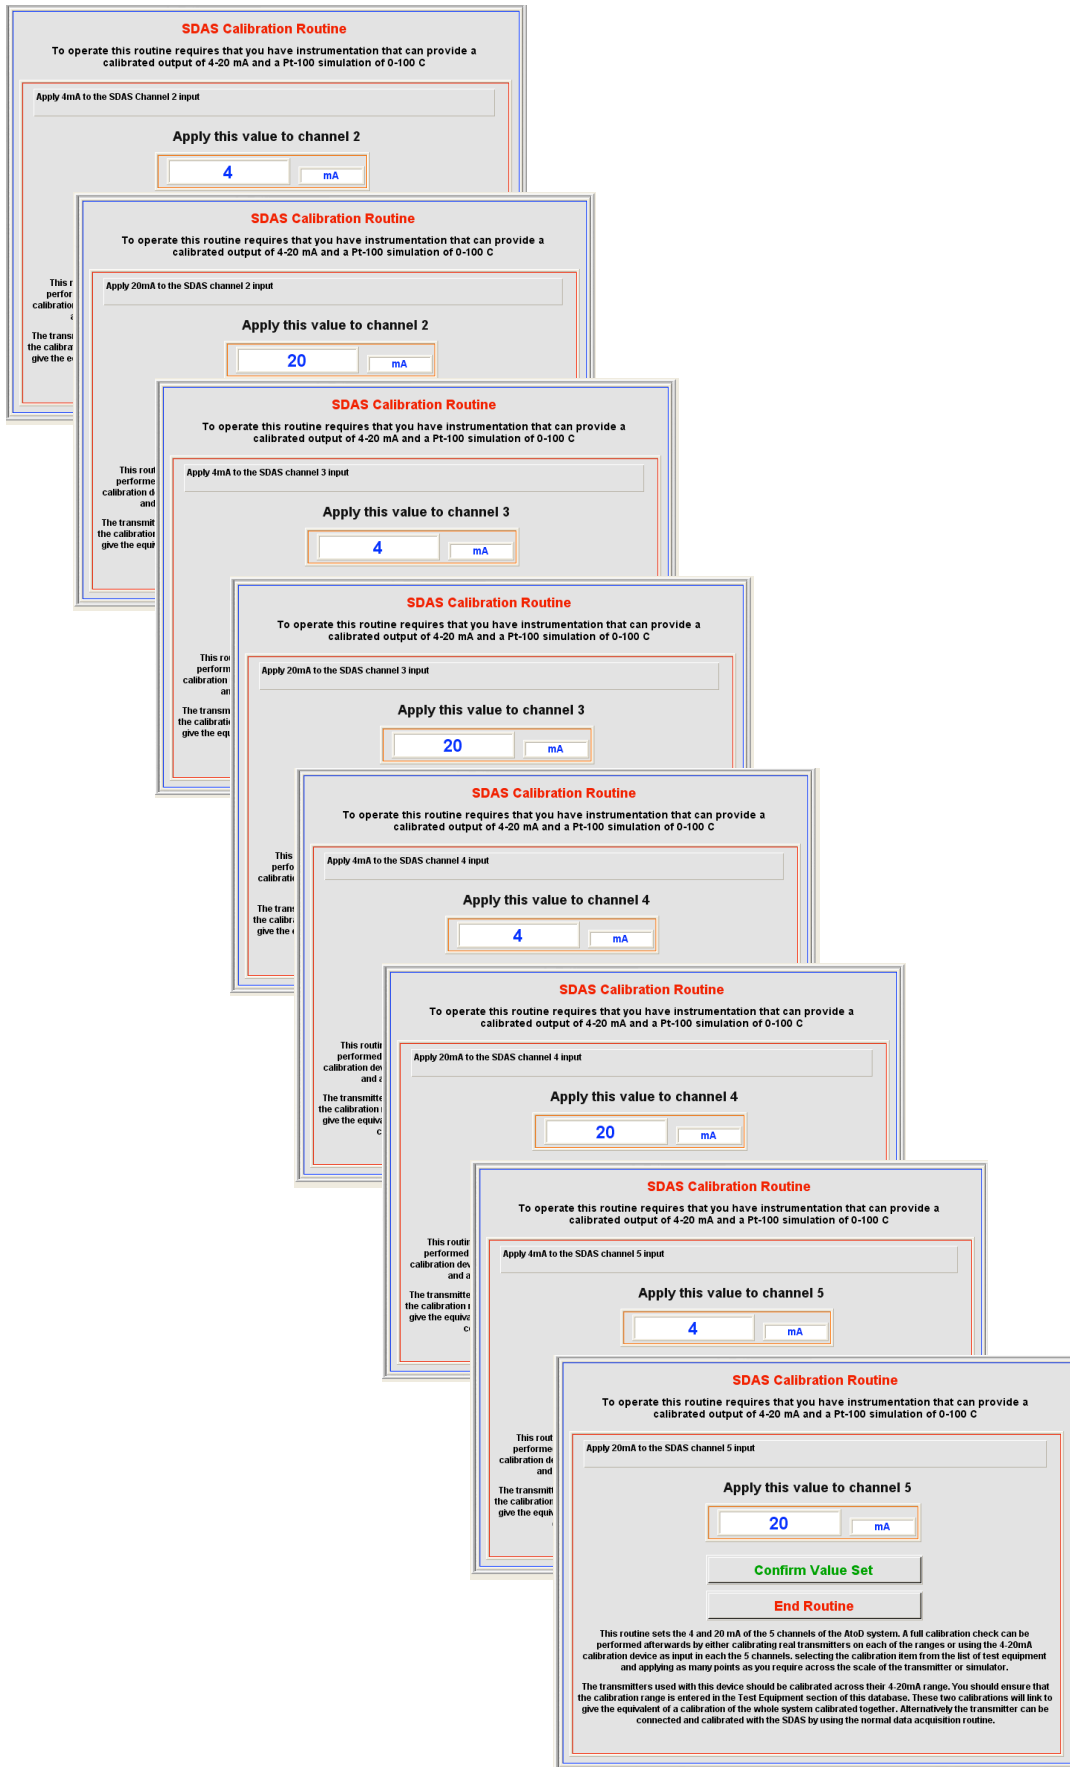


The SDAS unit I/O unit now performs a values check. If this ok then this screen appears and the unit is now calibrated.

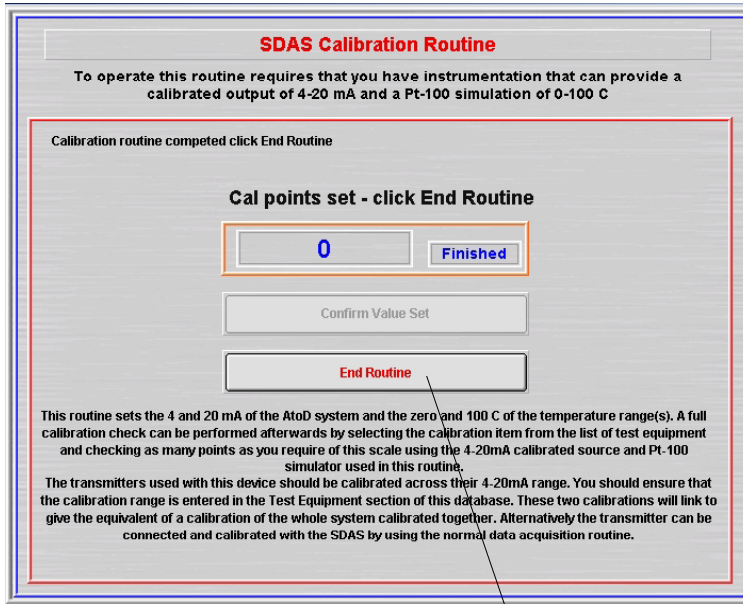


Click End Routine to exit the calibration

The values over the 4-20 mA and temperature ranges can be checked by providing input over the range using the calibration equipment and noting the values in the normal data gathering mode. A calibration certificate can be produced externally from these values.

If the SDAS I/O check gives an error then this screen appears. The SDAS I/O now may fail to operate correctly until an acceptable calibration is done.

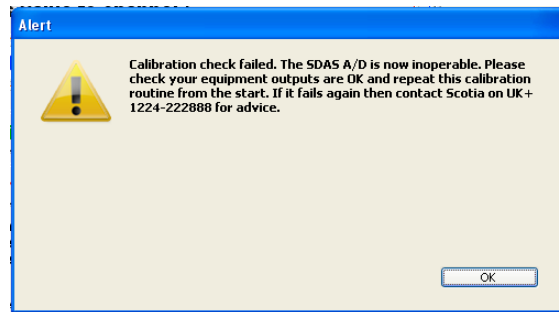


Get Connected Chip IDs

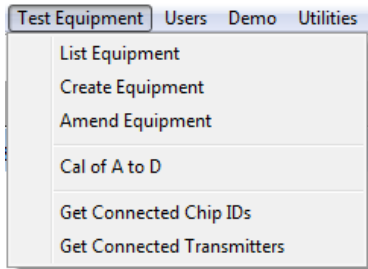

This routine gives the type and box chip ID of the SDAS unit and any connected transmitter chips in channel order. This allows the user to find the chip IDs for any Test transmitters or temperature entry.


The first 8 IDs are the transmitters connected to channels 1 to 8. This is followed by the chip IDs of the temperature probes. Only the SDAS5 uses chipped temperature probes.

The system then checks if the chipIDs are currently in the Equipment database. Any that are not in the database will fail when used so they should be added to the database before any data logging.

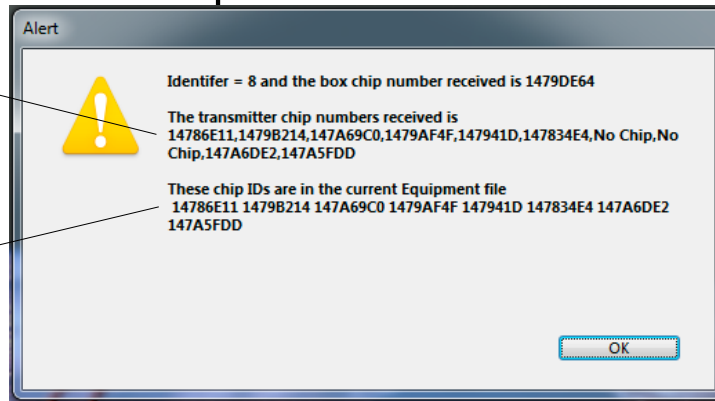

If any channels or temperature probes are either disconnected or do not have chipped items then this is shown as 'No Chip'.

Get Connected Transmitters

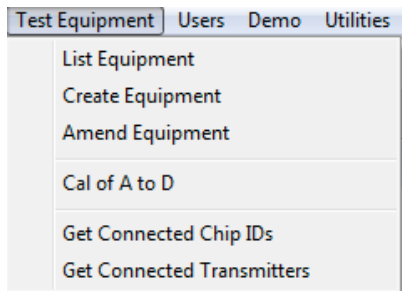

This routine gives the type and box chip ID of the SDAS unit and any connected transmitter chips in channel order. This allows the user to check what is connected with their range and calibration status. If the calibration due option is active then the current calibration status will be assessed.

Current Attached Equipment Status

These are the current Transmitters that are connected

		Channel Transmitters						Cal Date	ReCal Date
	Transmitter	Serial	Chip ID	Range					
Channel 1	Test CH1	S080558ch1	14786E11	0	700	bang	01/05/16	01/08/16	
Channel 2	Test CH2	S080558ch2	1479B214	0	750	bang	01/02/16	01/08/16	
Channel 3	Test CH3	S080558ch3	147A69C0	0	1000	bang	01/04/16	01/08/16	
Channel 4	Test CH4	S080558ch4	1479AF4F	0	1000	bang	01/05/16	01/08/16	
Channel 5	Test CH5	S080558ch5	147941D	0	1250	bang	01/05/16	01/01/17	
Channel 6	Test CH6	S080558ch6	147834E4	0	1900	bang	01/05/16	01/06/16	
Channel 7	Disabled	Disabled	Disabled	0	0	-	00/00/00	00/00/00	
Channel 8	Disabled	Disabled	Disabled	0	0	-	00/00/00	00/00/00	
		Temperature Probes							
Temp 1	Temp Probe	S080575T1	147A6DE2	0	100	seg C	00/00/00	01/01/17	
Temp 2	Ambient Temp	S080575T2	147A5FDD	0	100	seg C	00/00/00	01/06/17	

Proceed

User Menu

List Users

Users Demo Utilities Settings

- List Users
- Create User
- Modify Users
- Modify Level Access
- Change Current User

System User List

User ID	First Name	Last Name	Initials	Name	Status	Access Level
5	Calibration	Person	CP1	Calibration Person	Current	Level C
18	Demo	Person	DP1	Demo Person	Left	Level 5
4	QA	Person	QA1	QA Person	Current	Level Q
17	Review	Person	RP1	Review Person	Current	Level 3
2	Supervisor	Person	SP1	Supervisor Person	Current	Level 3
1	Test	Person	TP1	Test Person	Current	Level 1
3	Test	Person2	TP2	Test Person2	Current	Level 2
8	Administrator	Person	ZAP	The Administrator	Current	Level T

Finished

The list can be sorted ascending or descending by column by clicking the up or down arrow

This ends this routine


Double click on the user to view more detail

System User Entry

Enter the user details below. The 'User Name' entry is how the user will appear on the selection list and the 'Initials' entry is what is used as the person identifier.

First Name
Last Name
Initials
User Name
Password
Access Level
System Group
Status

Create User

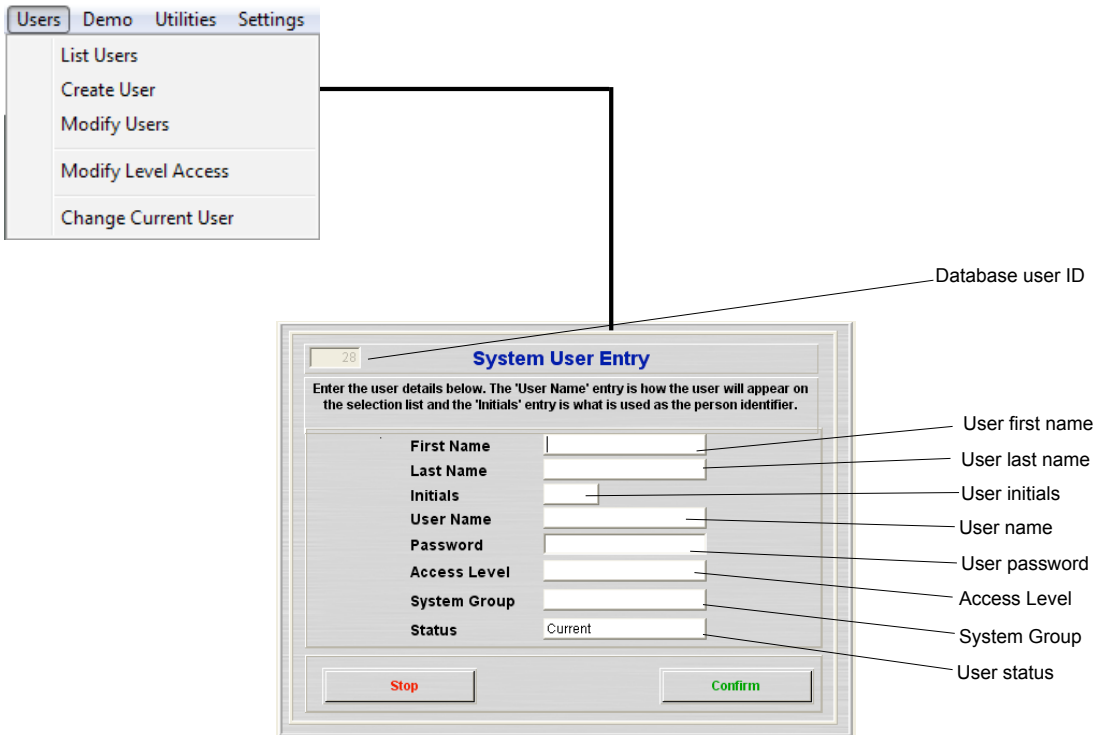

The user first and last name can be entered as anything. This is copied to the User name. The user name can then be adjusted to allow for the user being 'known' as something different. The User Name is what appears on selection lists. The initials are database unique and must be entered as 3 alphanumeric characters. If these exist in the database then you are alerted and must choose other initials. These are used to identify the user in the data label system. Password can be any alphanumeric. Access Level allows this user the access set in the Access Level system. System Group is the group of users that access the system using the entry password when the SDAS is started. Status is the current status of this user. Only users with status 'Current' will appear on the selection pop-up list and be able to log in.

An example of a completed entry

The image shows the 'System User Entry' dialog box with a completed entry. The title bar shows '16' and 'System User Entry'. Below the title bar is the same text box: 'Enter the user details below. The 'User Name' entry is how the user will appear on the selection list and the 'Initials' entry is what is used as the person identifier.' The form contains the following fields:

- First Name: Demo
- Last Name: Person
- Initials: DP1
- User Name: Demo Person
- Password: (empty)
- Access Level: Level 5
- System Group: -User1
- Status: Current

At the bottom of the dialog box are two buttons: 'Stop' and 'Confirm'.

Modify Users

Users Demo Utilities Settings

- List Users
- Create User
- Modify Users
- Modify Level Access
- Change Current User

System User List

User ID	First Name	Last Name	Initials	Name	Status	Access Level
5	Calibration	Person	CP1	Calibration Person	Current	Level C
16	Demo	Person	DP1	Demo Person	Left	Level 5
4	QA	Person	QA1	QA Person	Current	Level Q
17	Review	Person	RP1	Review Person	Current	Level 3
2	Supervisor	Person	SP1	Supervisor Person	Current	Level 3
1	Test	Person	TP1	Test Person	Current	Level 1
3	Test	Person2	TP2	Test Person2	Current	Level 2
6	Administrator	Person	ZAP	The Administrator	Current	Level T

Finished

The list can be sorted ascending or descending by column by clicking the up or down arrow

This ends this routine

Double click on the user to view more detail

System User Entry


Enter the user details below. The 'User Name' entry is how the user will appear on the selection list and the 'Initials' entry is what is used as the person identifier.

First Name
Last Name
Initials
User Name
Password
Access Level
System Group
Status



Do not make any changes

Confirm any changes

Modify Level Access

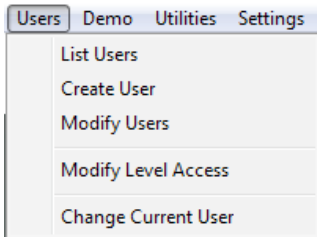

Access to this menu item is restricted. If the user does not have access then this screen appears

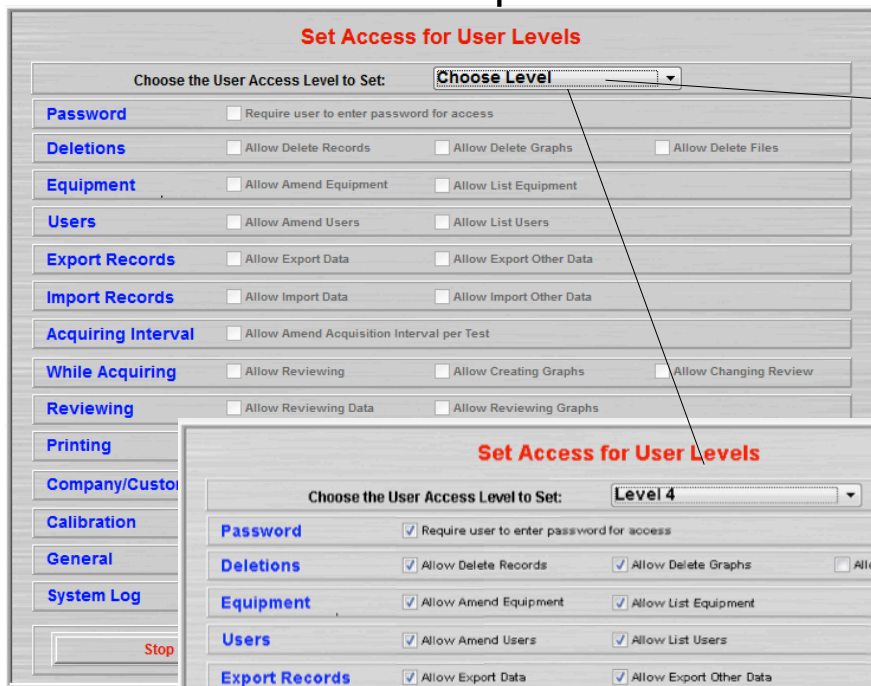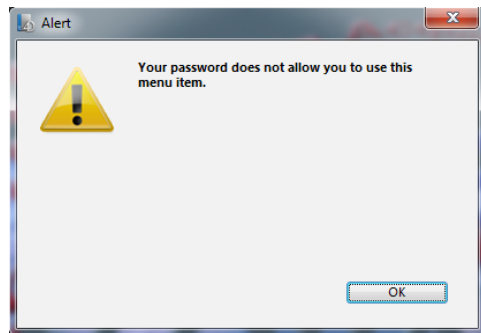

Choose the Access Level to be altered from the pop-up list



When the Access Level is chosen the permissions set for that level are shown. They can then be set or unset by clicking on the box beside each item.

Revert to the previous settings

Confirm to accept the changes made

Access Levels:

Password: The user is required to enter a password to log on. If not checked the user does not require a password.

Deletions: Allow the user to delete data, graphs or files when the file browser option is enabled.

Equipment: Allow the user to enter or amend the testing equipment file. Allow the user to see the list of testing equipment.

Users: Allow the user to enter or amend the system user list. Allow the user to see the list of users.

Export Records: Allow the user to Export Data and Graphs. Allow the user to export other data e.g. user lists.

Import Records: Allow the user to Import Data and Graphs. Allow the user to import other data e.g. user lists.

Acquiring Interval: Allow the user to set the acquiring interval before each data acquisition.

While Acquiring: This limits what the user can do while actually acquiring data. Allow Reviewing allows the user to access the Review screen from the acquiring screen. Allow creating graphs - with access to the Review screen the user can create graph files. Allow changing Review - with access to the Review screen the user can choose to view another data file.

Reviewing: Allow the user to access the Review Data menu item. Allow the user to access the Review Graphs menu item.

Printing: Allow the user to print data listings.


Company/Customer: Allow the user to set the Company name. Allow the user to set the default Customer name.

Calibration: Allows SDAS calibration. Restrict access to this as inexperienced use of this routine may render the SDAS inoperable.


General: Allow the user to set the default acquiring interval. Allow the setting of the default Comms port - this is to allow the SDAS program to be used on a PC which may access a remote unit via another port. Restrict access to this as inexperienced use of this routine may render the SDAS inoperable. Allow setting logo - allows the user to load up a new logo for appearing in the printed graphs.

System Log: Allows users to view the system log


If access is denied due to a user not having a high enough Level access for any menu items then this screen appears.

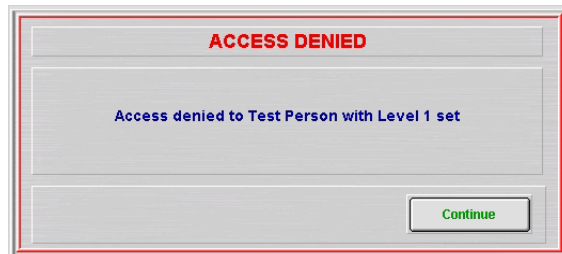


If access is denied due to a user not being in the correct log on Group for this action then this screen appears.

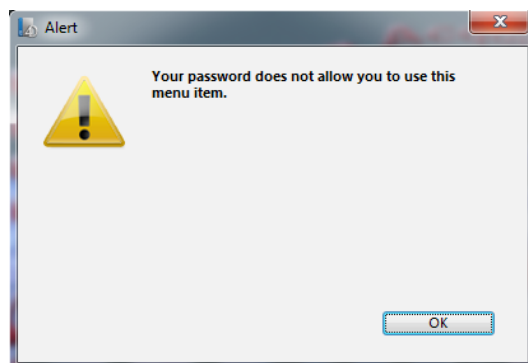

Change Current User

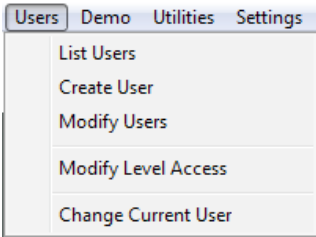

This allows the current user to be changed without restarting the SDAS system.

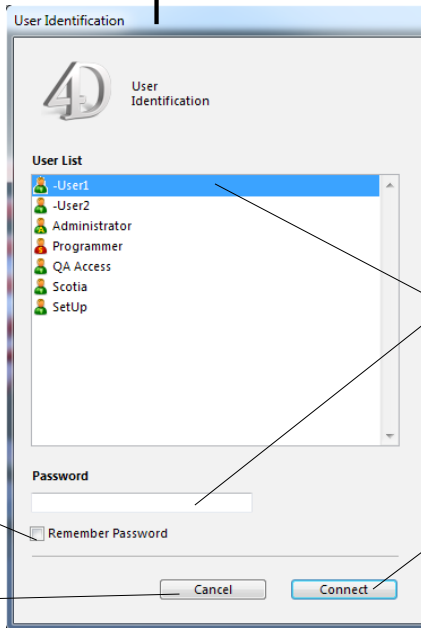

Choose the User Group access name and enter the User Group password here

Do NOT choose to have the system remember the group password


Cancel returns to the main screen with the previous user reset

Confirm to proceed to user name and password entry



Choose the user name from the pop up list here

Only user names in the Access Group chosen above will appear in the pop up list for choosing.

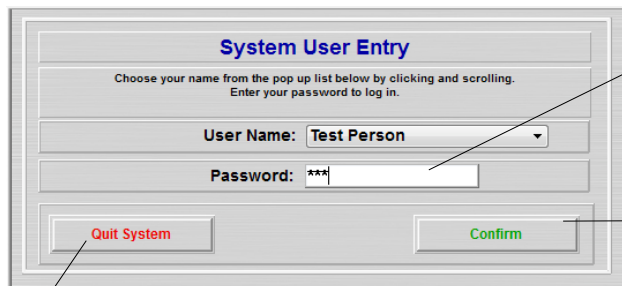


When the name has been chosen you enter the password for this user. The entry does not show for security

Confirm to proceed back to the main screen with the new user.



If you do not have a valid user password then Quitting from the SDAS program is the only other option at this point.

Utilities


Print Setup

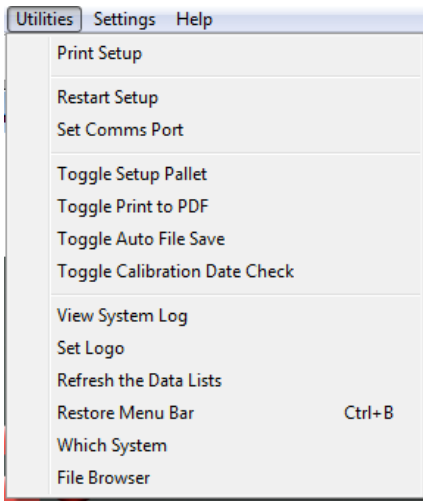

This checks the printer settings

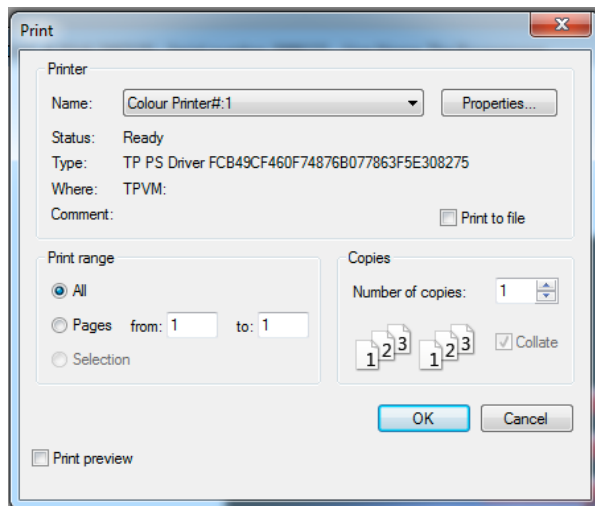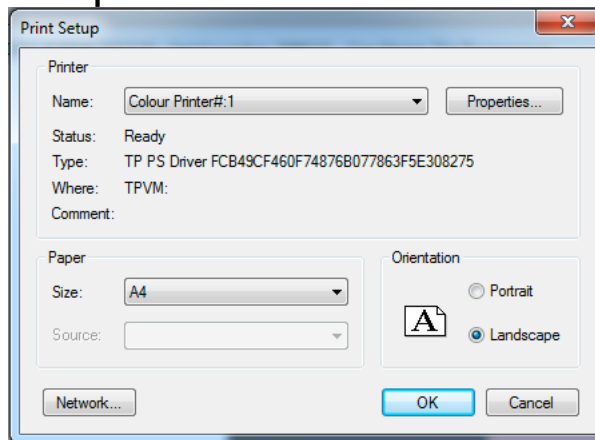


Restart Setup

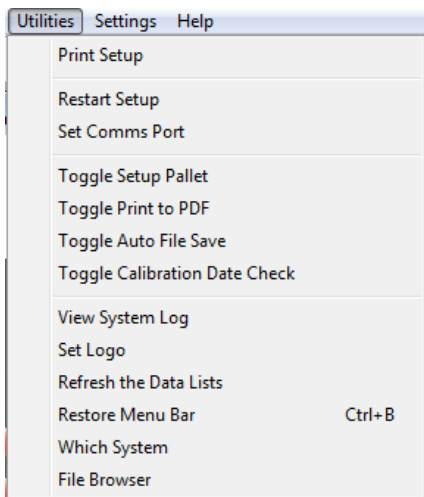


This runs the start up routine for the SDAS6 program. In most cases this has the same result as shutting down and restarting except it may not reset any other connected component.

Set Comms Port

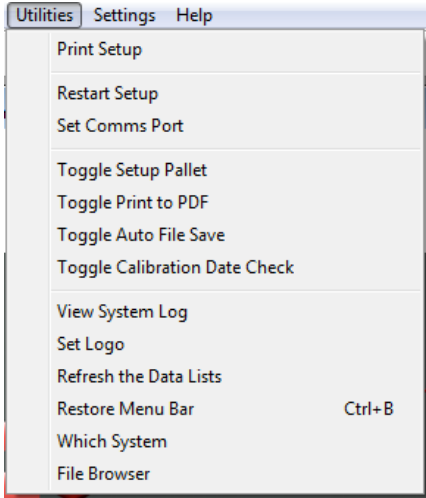

The communications setting between the components of the SDAS system can be set here. Setting the system wrongly will stop the system. A restart will restore the settings originally set by Scotia.

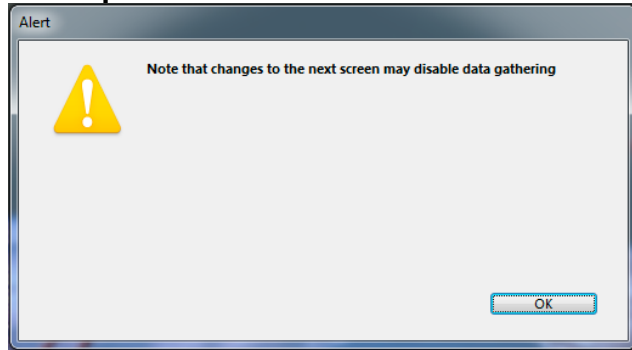


This sets which port to use when the computer has a serial port

This sets the time out - the system will wait this many seconds before deciding it has a comms failure

This sets the handshaking system


Stop without making any changes

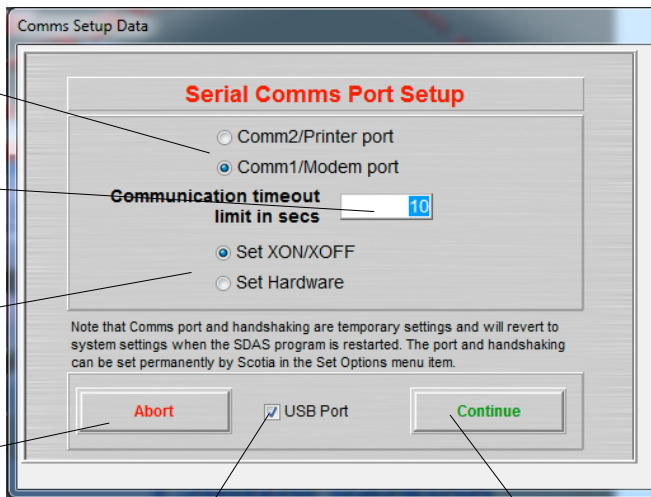

If the port used is the USB port then this should be checked

Confirm the setting and continue


Toggle Setup Pallet

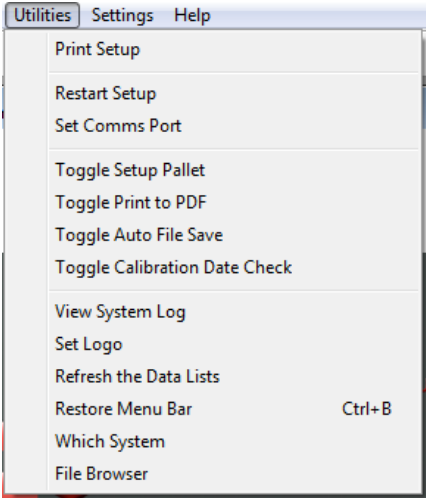


When the Setup Pallet is enabled it may be the user does not want to use this option where the test being done does not require it. When toggled to off the normal SDAS operation is done avoiding all the setup screens.

The Setup Pallet is the inactive until this routine is ran again to turn it on.


If this option is not enabled you get a message to say that

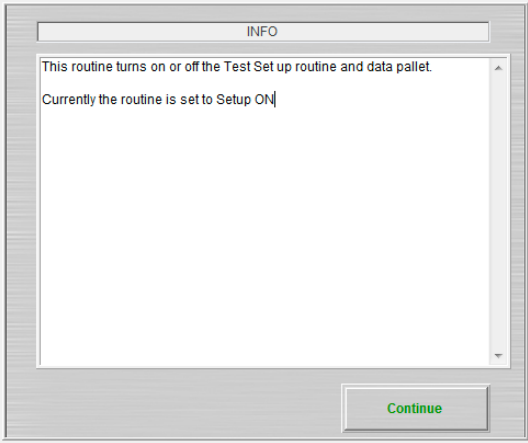


Choose to change the current setting or not

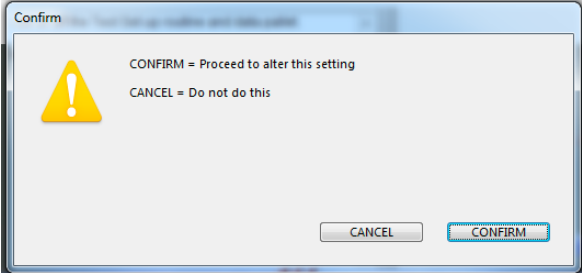


Set this on or off

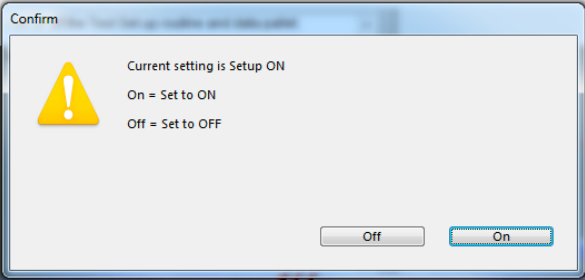


Toggle Print to PDF

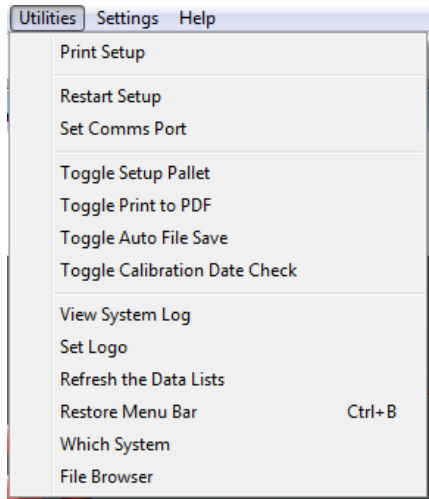


The system can be set to print to printer or PDF
 If set to PDF the file will be saved in the Default Saving folder

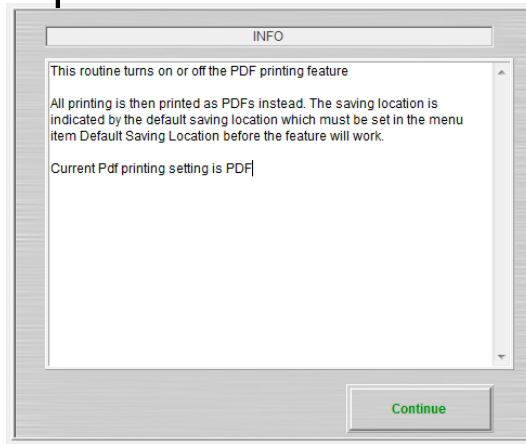


Choose to change the current setting or not

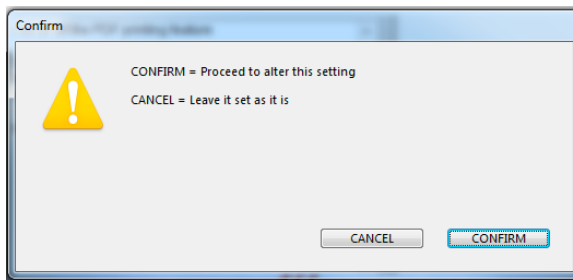

Set this to printer or PDF

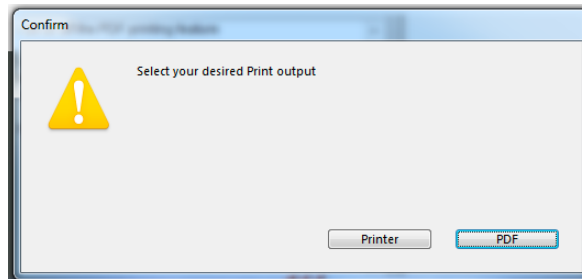


Toggle Auto File Save

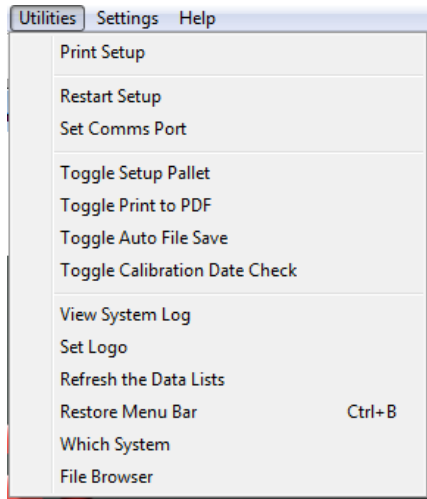


With this option on this toggles the saving of a secure data file to the default saving location when the Finish button is clicked at the end of a test.


If this option is not enabled you will get a message to say that

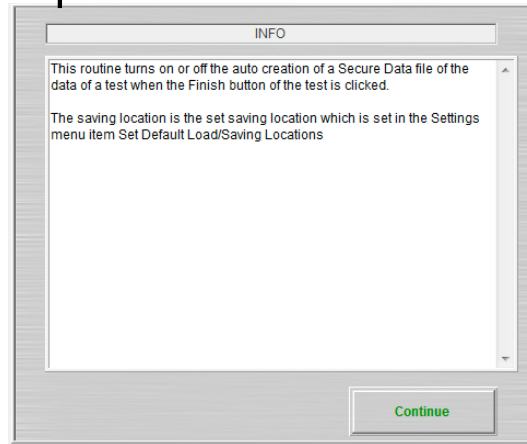


Choose to change the current setting or not

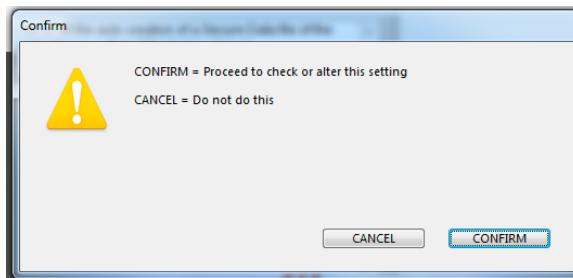

Set this to On or Off

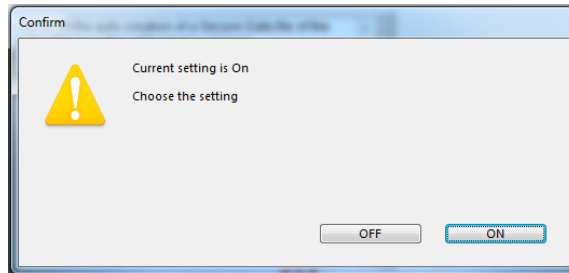


Toggle Calibration Date Check

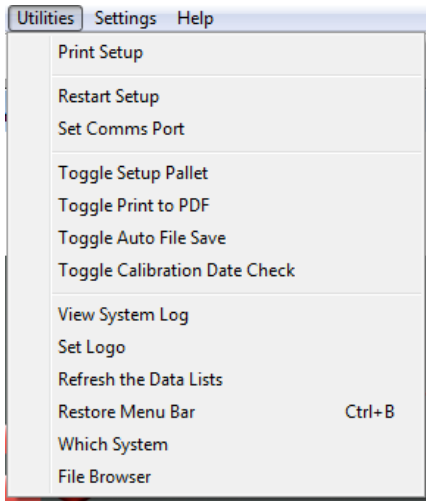


With this option toggled on the system checks the calibration due date of any connected transmitters or temperature probes before a test is started. Any items that are due calibration will report that and the test cannot proceed.


If this option is not enabled you will get a message to say that

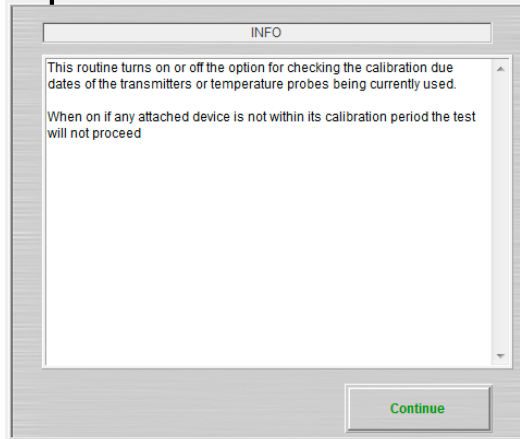


Choose to change the current setting or not

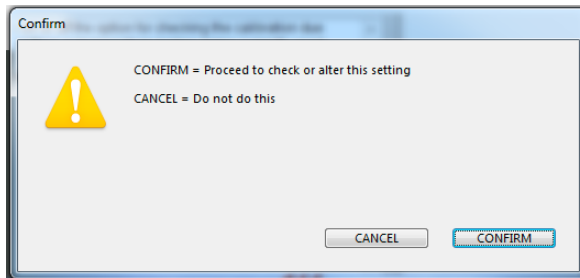

Set this to On or Off

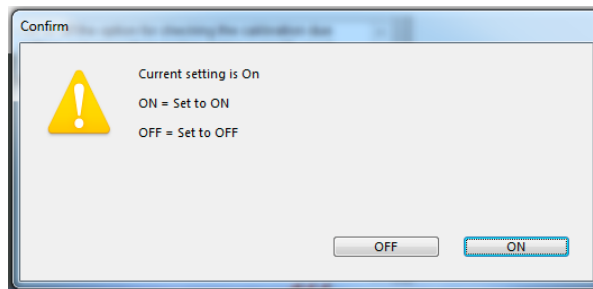


View System Log


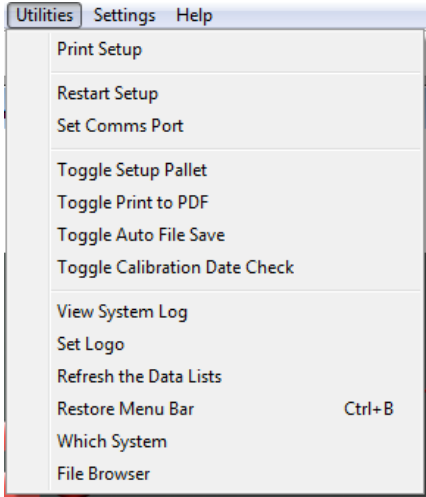


The System logs can be viewed here

Clicking on Choose Log File gives a drop down list of the files available




The number of files expands as the data stored increases. LogAccess1 shows who has logging and out of the system. LogAction is the log of changes to the system. LogAError1 is the log of any system problems.

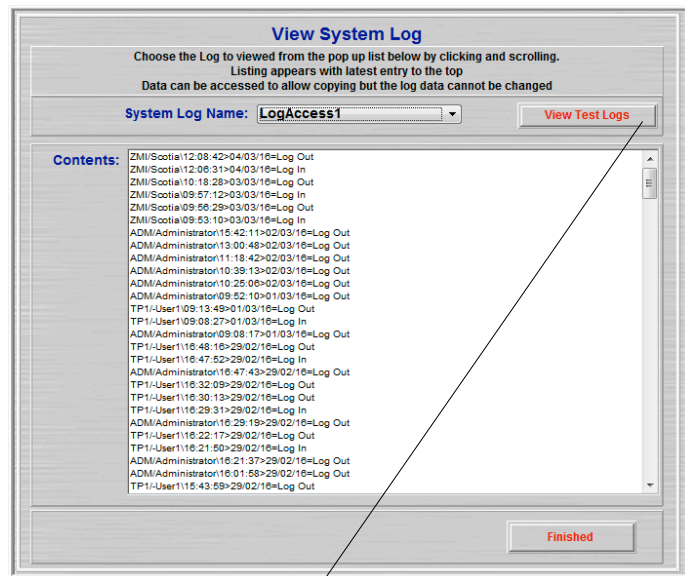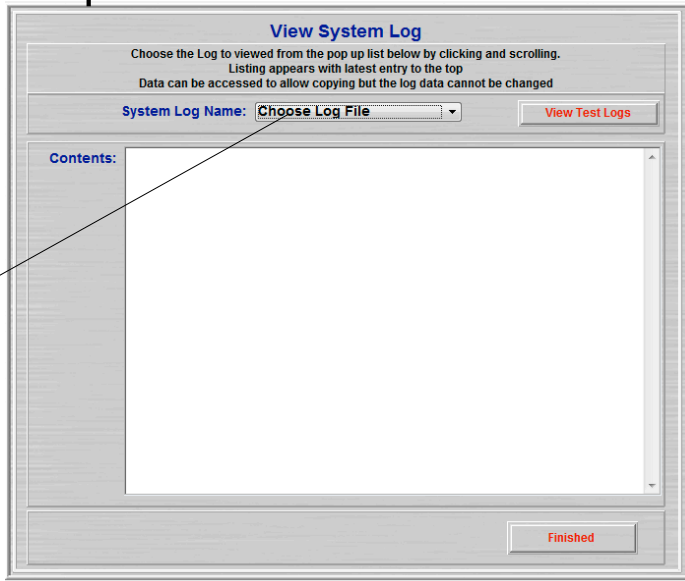


View Test Logs appears if the Test Event Log option is active.

Each test has its own Test Log stored - even if this option is not enabled. With this option on the user gets to view the Test logs


When View Test Logs is clicked then this screen appears

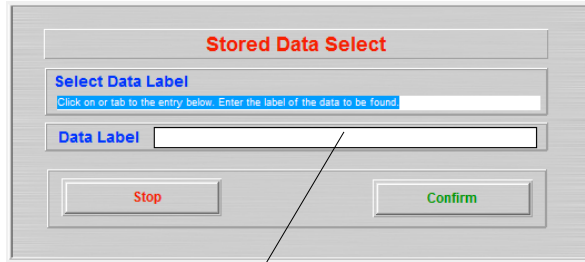

Click to bring up a list of the test logs in the system

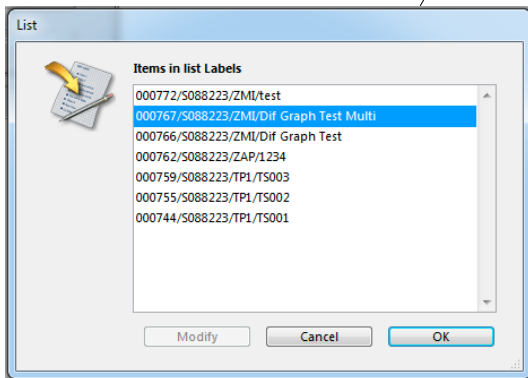


Click on one to select it and click OK

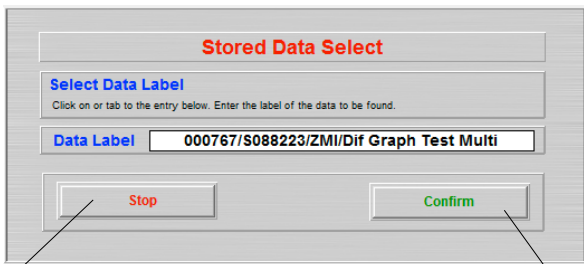


The Data Label selected is entered for the search

Stop to finish

Confirm to proceed to show this test log

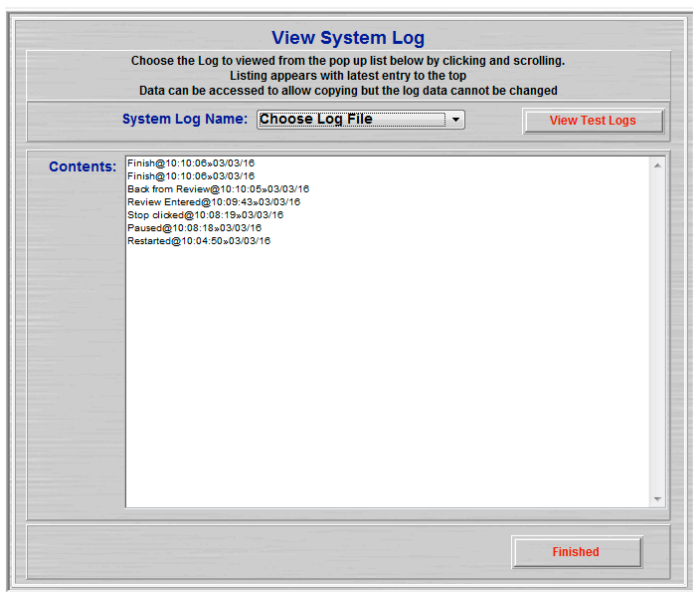

Set Logo

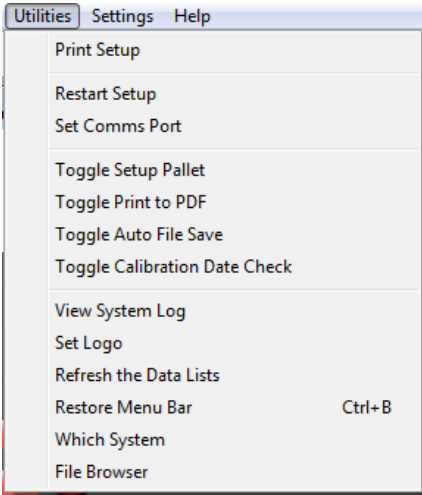


This allows the logo for the graph printing to be reset by importing a graphic.

The graphic to be imported should be square or it will distort when displayed. The logo should be saved to storage media in jpg form. This is then found by the normal PC load routine after clicking the Load Logo button.

The other way is for the logo to be captured to the clipboard of the PC in the usual way. Then click on the existing logo graphic and paste your new graphic. If the graphic is too small or not square some distortion may occur.

The first method gives the most reliable results.

If you do not have a graphic of your logo either leave the existing one or replace it with a 'blank' graphic.

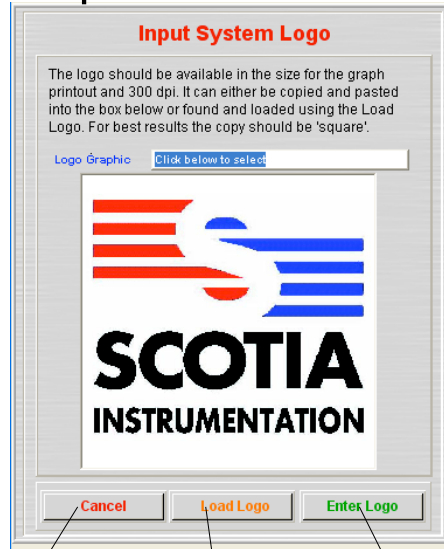


To set the SDAS to have no logo click on the current logo to select it and then press the delete key

Do not make any changes here

Navigate to the logo you wish to import.



Confirm the entry

Refresh the Data Lists

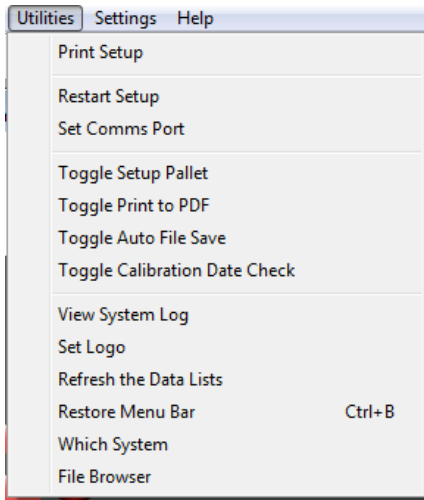


If you find the list of Data Files does not include a file which you know should be there then this routine refreshes the choice lists. Problems like this are generally caused by the SDAS routines being interrupted by power loss etc.

When using the Review version and importing data you get the option to delay rebuilding these lists. This can be used if you change your mind.

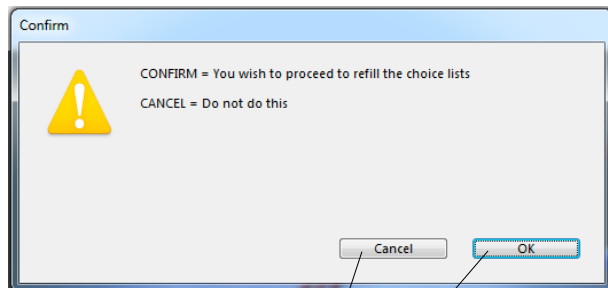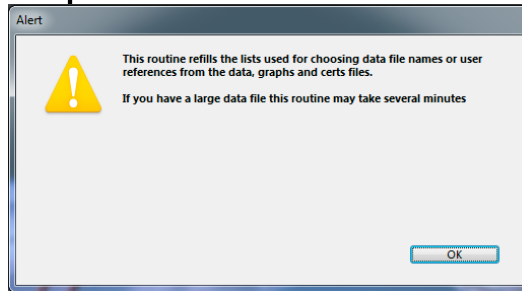

Do not do that Rebuild the data lists


Restore Menu Bar

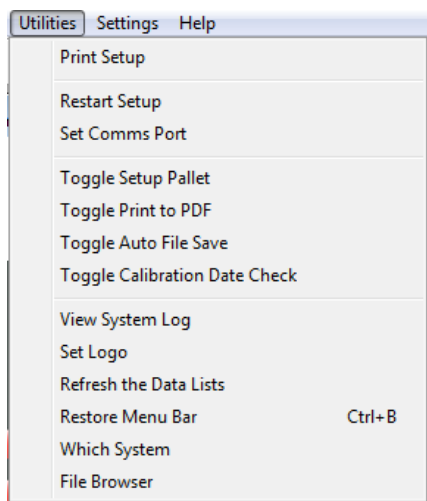

The menu bar is removed once a menu item has been selected to avoid the user trying to select it while operation screens are active. Should a system error occur then the SDAS may reset to the start screen but not showing the menus.


In this case this menu and menu item will not be visible either but it can be activated by holding the Control key down and pressing the B key. Once this is restored then you should go through the close down routine of the SDAS unit, switch off the SDAS, and then restart to ensure all the other linking electronics have reset correctly.

Which System

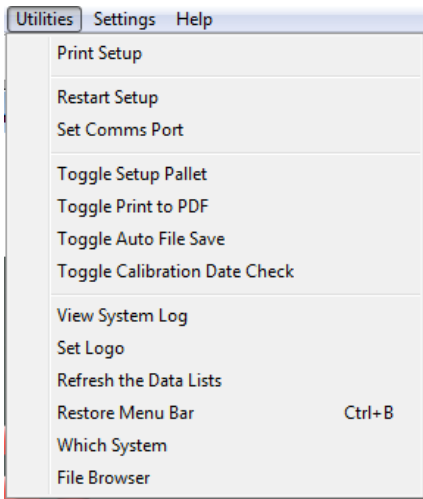

This is included for debugging purposes as certain components of this structure operate differently in different systems. This is just checking the SDAS program is resolving this data correctly.

File Browser

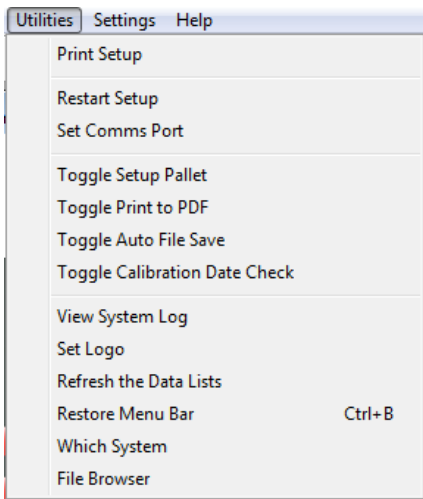


From SDAS v6.09 control of deletion of SDAS externally saved files has been passed to the program from the operating system. Deletion is allowed from the Levels setting for Users.


The externally saved files in the four set locations can be copied, moved and deletion using the following screen.

Network folders can be seen and copied to but cannot have any other actions to them.

The screen opens like this

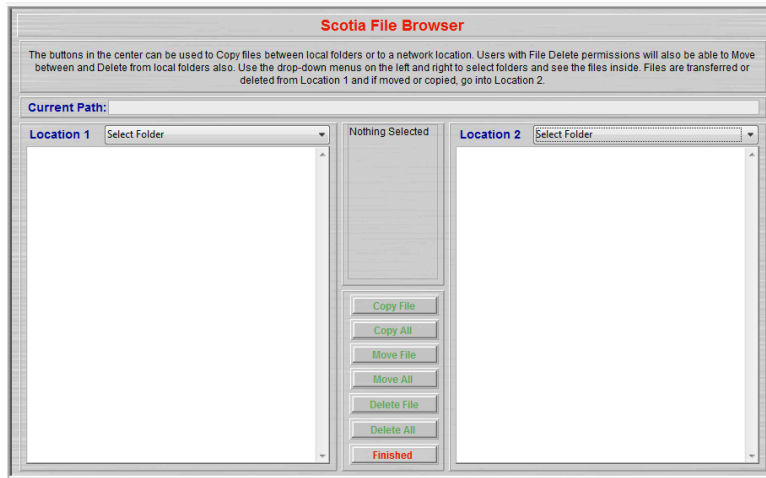


Pick the source folder from the list offered

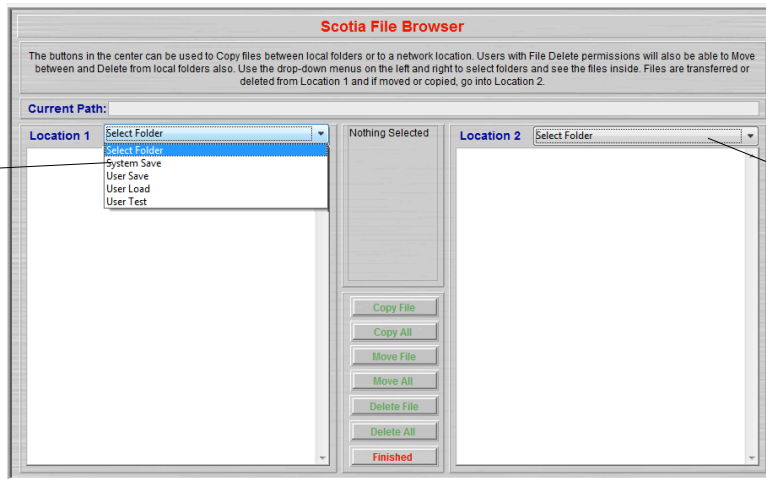

Pick the target folder from the list offered

The list of available files are shown listed here. Scroll if there are more than can be seen. Click on the one required to select it. The path to this file is shown above.

If the file is not local to the SDAS you cannot copy, move or delete from that folder.

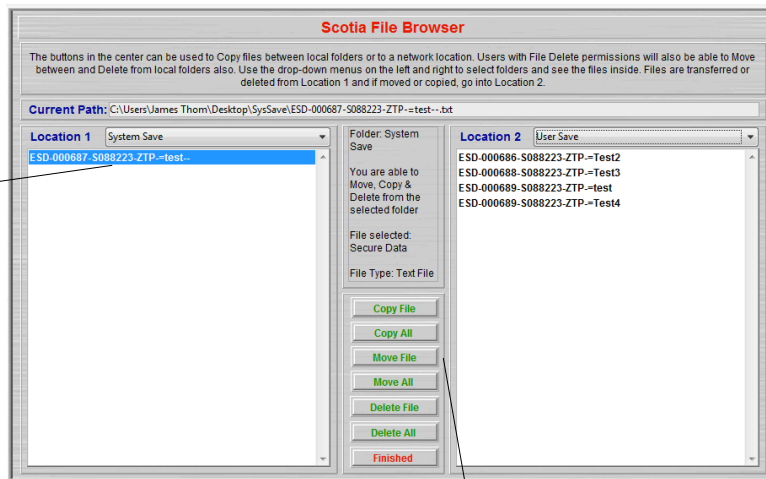


All users can copy from a local folder but can only move and delete if they have permission set in their Levels.


These buttons activate according to what is allowed

Settings Menu

Set Company Name

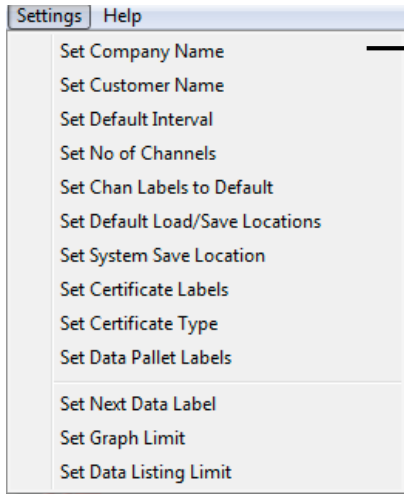

This sets the company name that appears on graph capture screens and prints. This can only be set here.

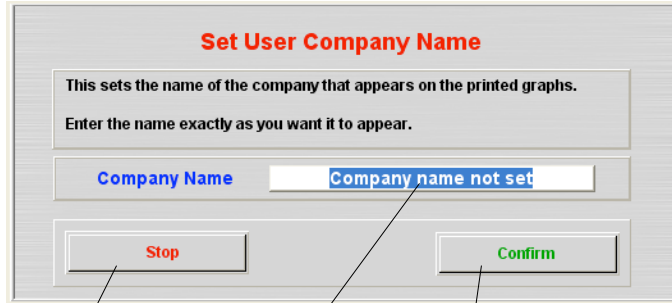


This leaves the name unchanged


Enter the name required here

This confirms the change of name

Set Customer Name

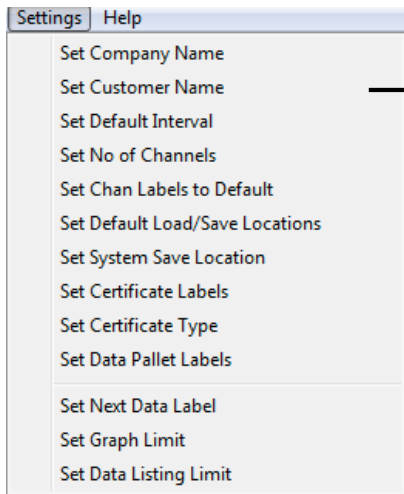

This sets the customer name that appears on graph capture screens and prints. This can also be entered or changed at the Graph screen

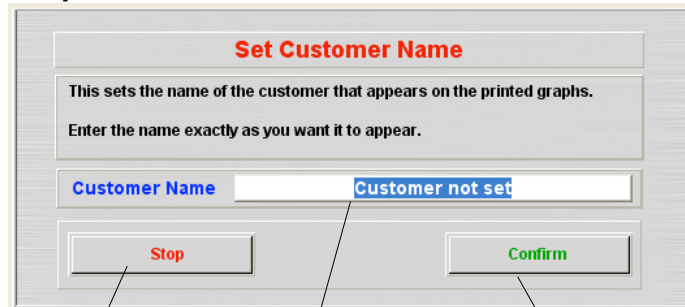


This leaves the name unchanged


Enter the name required here

This confirms the change of name

Set Default Interval

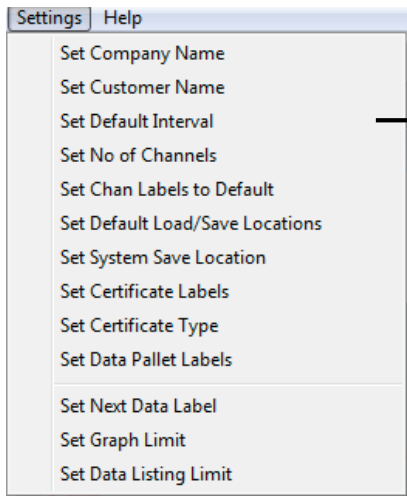

This sets the default time interval for acquisition in seconds. If you test regularly at a certain time interval then this could be set here. The interval can be set again at the start of any test.

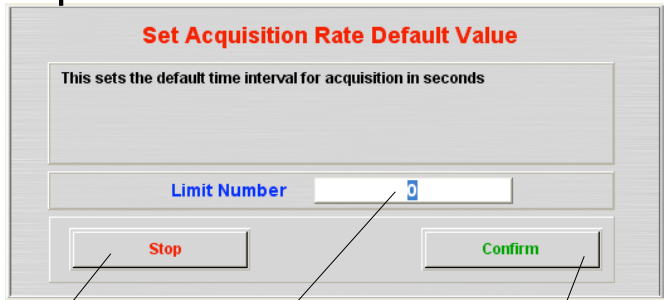


This leaves the setting unchanged

Enter the new value here. Note that zero means log as fast as possible which is currently every second


This confirms the change

Set No of Channels

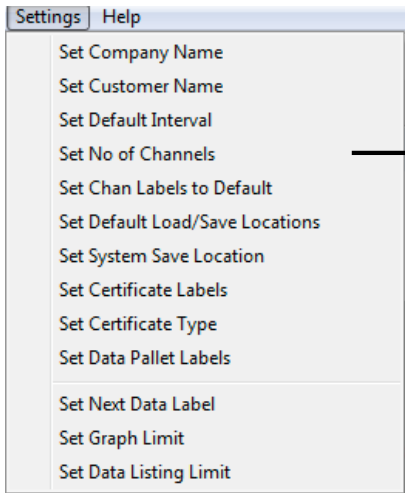


Access to this menu item is restricted as altering this may not be obvious to a user and will restrict the number of channels operating

In multichannel SDAS units this allows the number of active channels to be set. If you only use the SDAS on 3 channels then setting 3 channels here will prevent you having to turn those channels off or remove any attached transmitters when starting tests. Note that the active channels count up from channel 1. In the case of 3 active channels these are always channels 1,2 and 3.


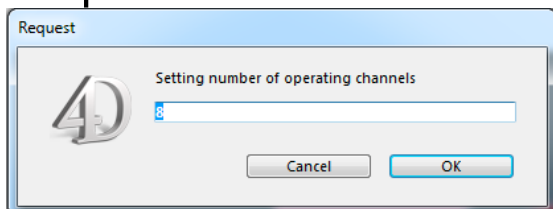


Channels above the number set are disabled and cannot be used even if a transmitter is attached

Set Chan Labels to Default

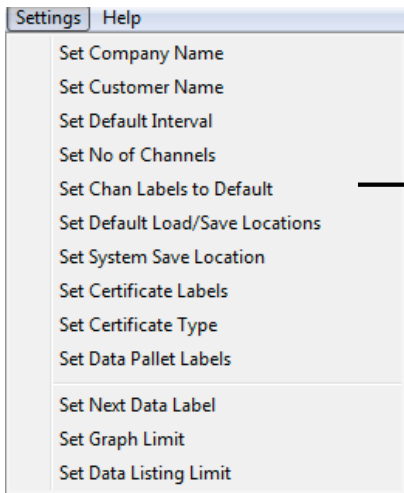


The channel labels can be set by the user to make the channel names more meaningful. This routine allows these to be reset to Trans1 to Trans8

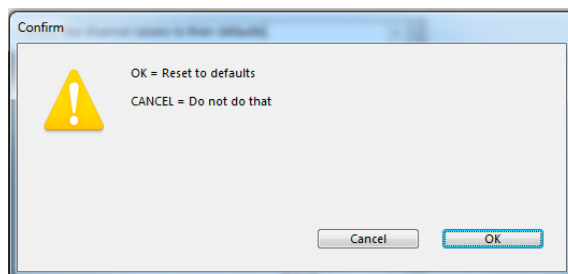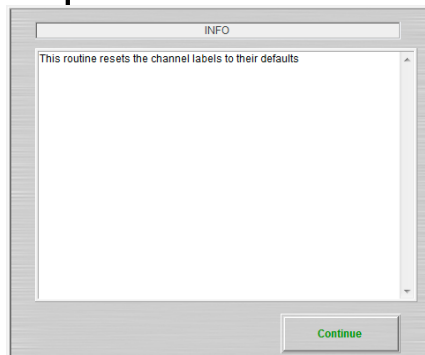

Ok restores the default values


Set Default Loading Location

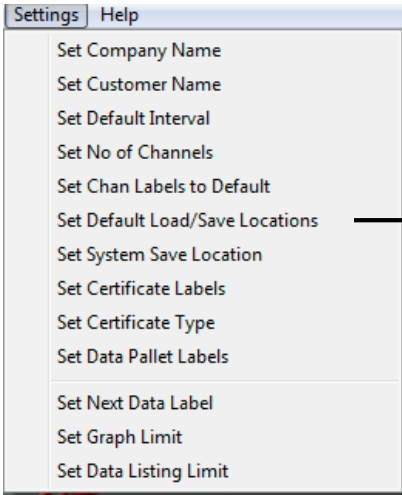

This sets the location for the system to save/load files. The location can be the main drive, external saving media or a network location

This menu item is only accessible by users logged in as QA Access as setting this incorrectly will stop certain functions.

Note that clicking on the buttons to search for a folder and then not proceeding will blank the path. Clicking Don't Save will restore the path if you then restart the SDAS. Do not tamper with this screen unless you know what you are doing.

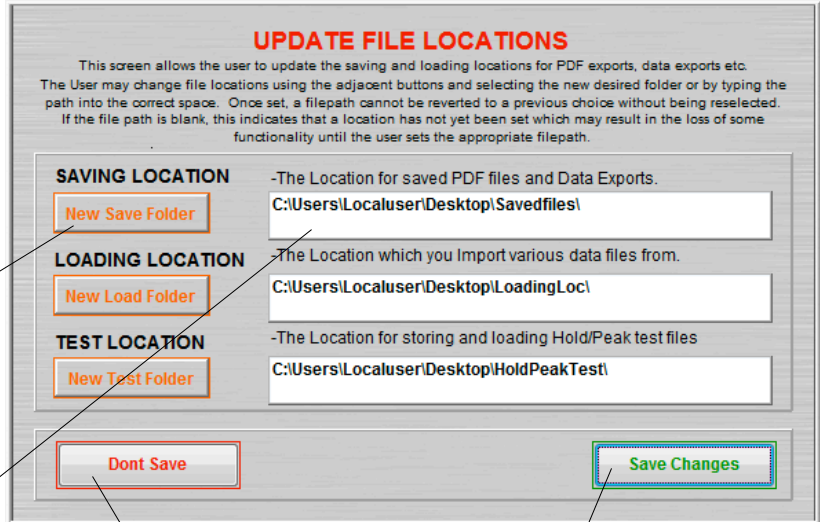


Clicking on these buttons opens a system browser to allow you to navigate to the folder required. This can be local to the SDAS, a USB stick or a network location.

The path to that location is then inserted into the path box

The path can be entered manually here. The path is checked for validity as you exit the field

This does not save any changes to the loading routine

This confirms the change and saves the settings

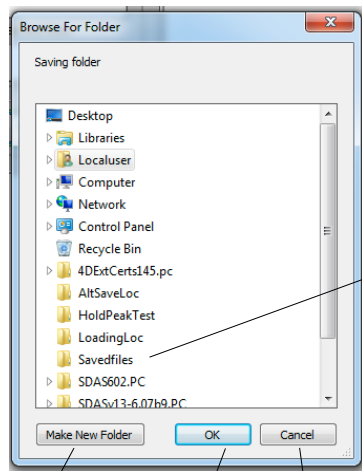


Choose the folder to set here by clicking once on it

A new folder can be created and named here

Click OK to confirm

Clicking Cancel will set a blank path


Set System Save Location

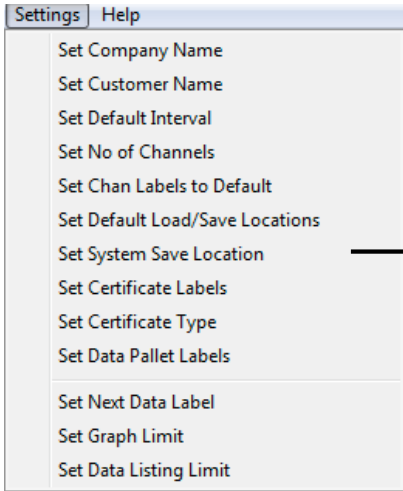

This sets the reserve location for the system to save files. The location chosen should ONLY be a local folder. This is the location files are saved when the normal saving location cannot be found.

This menu item is only accessible by users logged in as QA Access as setting this incorrectly would stop certain functions.

Note that clicking on the buttons to search for a folder and then not proceeding will blank the path. Clicking Don't Save will restore the path if you then restart the SDAS. Do not tamper with this screen unless you know what you are doing.

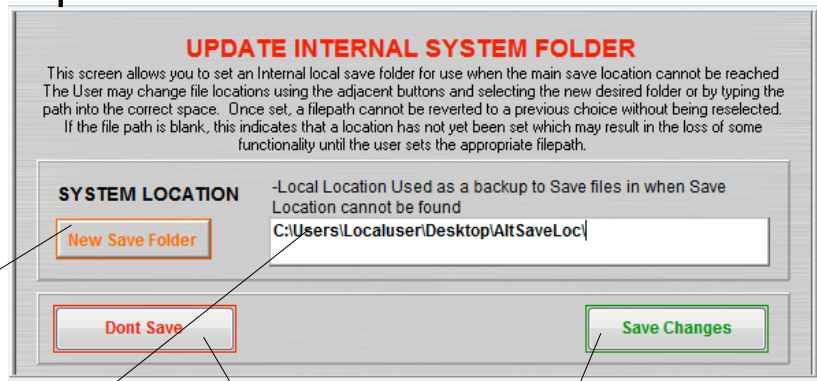


Clicking on this button opens a system browser to allow you to navigate to the folder on the local drive.

The path to that location is then inserted into the path box

The path can be entered manually here. The path is checked for validity as you exit the field

This does not save any changes to the loading routine

This confirms the change and saves the settings

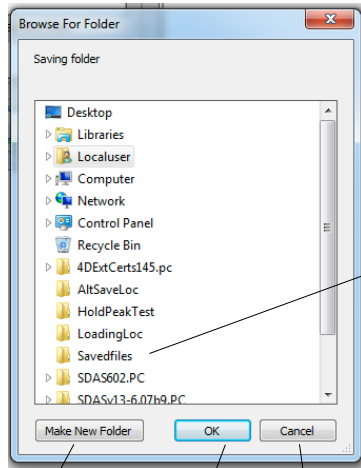

Choose the folder to set here by clicking once on it

A new folder can be created and named here

Click OK to confirm

Clicking Cancel will set a blank path

Set Certificate Labels

Settings Help

- Set Company Name
- Set Customer Name
- Set Default Interval
- Set No of Channels
- Set Chan Labels to Default
- Set Default Load/Save Locations
- Set System Save Location
- Set Certificate Labels
- Set Certificate Type
- Set Data Pallet Labels

- Set Next Data Label
- Set Graph Limit
- Set Data Listing Limit

With the certificates option active the labels on the certificate can be set to ones chosen by the user. These labels are saved with the certificate so changes made at a later date do not affect certificates already done.

All labels with a white background can be set by the user

Test Inspection Certificate Labels

This sets the labels for this test certificate - Enter or change the Label Details below

Type 1

Certificate Title: Hydrostatic Test Inspection Certificate

Issuing Company: A Customer

Issuing Coy Address: Issuing company address

Client Name	
Client Contact	
Client Job Number	
Our Job Number	
SDAS User Reference	
SDAS Data Label	
Drawing No(s)	
Spool No(s)	

Location	
Test Type	
Test Pressure	
Test Medium	
Test Duration	

	Time	Date	Pressure
Test On			
Test Off			

SDAS Serial Number	
Pressure Transmitter	
Range	
Traceable Standard	
Pipewall Temperature Probe Serial No	
Our Company	

Set Certificate Type

Settings Help

- Set Company Name
- Set Customer Name
- Set Default Interval
- Set No of Channels
- Set Chan Labels to Default
- Set Default Load/Save Locations
- Set System Save Location
- Set Certificate Labels
- Set Certificate Type
- Set Data Pallet Labels

- Set Next Data Label
- Set Graph Limit
- Set Data Listing Limit

Two different types of certificates are stored in the system. With this option on choosing here sets the one to be used.

Request

Enter the certificate type to use (1 or 2)

Set Data Pallet Labels

Settings Help

- Set Company Name
- Set Customer Name
- Set Default Interval
- Set No of Channels
- Set Chan Labels to Default
- Set Default Load/Save Locations
- Set System Save Location
- Set Certificate Labels
- Set Certificate Type
- Set Data Pallet Labels
- Set Next Data Label
- Set Graph Limit
- Set Data Listing Limit

With the Data Pallet option active the labels on the Data Pallet can be set to ones chosen by the user. These labels are saved with the test data so changes made at a later date do not affect tests already done.

The data pallet labels can be set by the user


Data Pallet Setup Labels

This sets the labels for the Setup screen for the data pallet - Enter or change the Label Details below






Sales ONo	
Work ONo	
Part No	
Serial No	
Proc No	
Proc Section	
Cust Name	
Operator	
Inspector	

Stop Confirm


Set Next Data Label

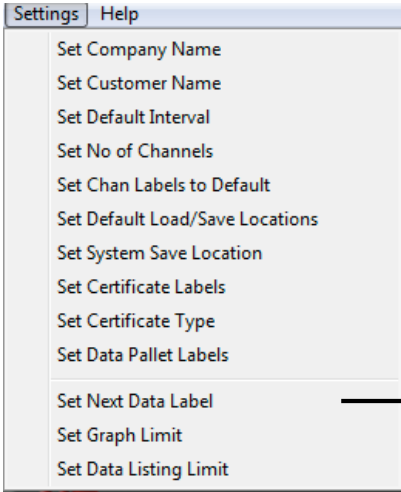

The tests are labelled with test identifier. It may be necessary to reset this number so this routine was added for that purpose. You need to be sure you have a good reason to do that.

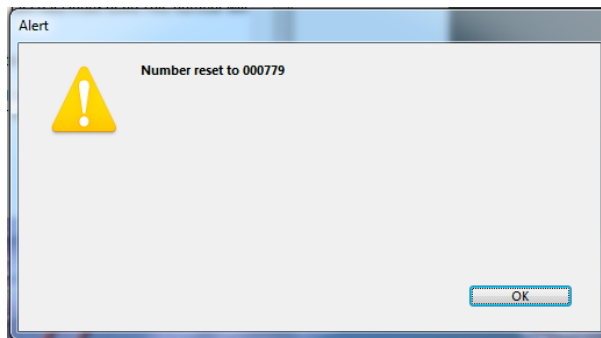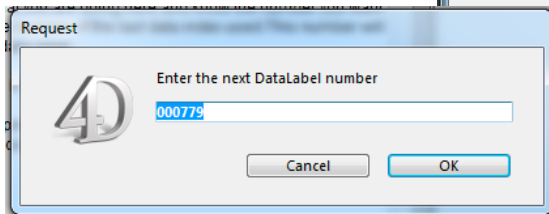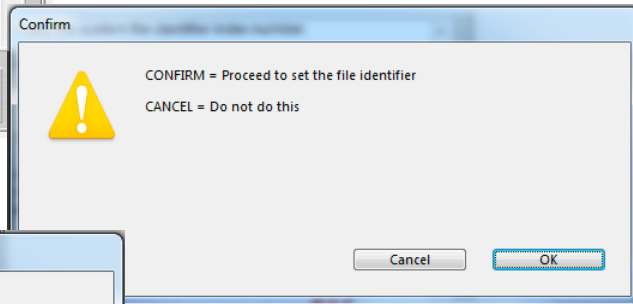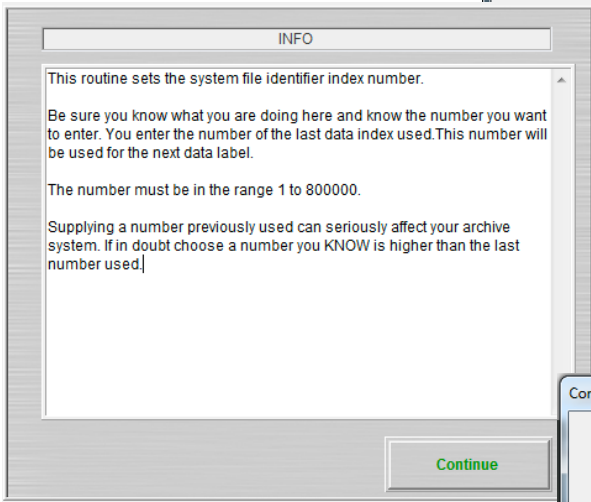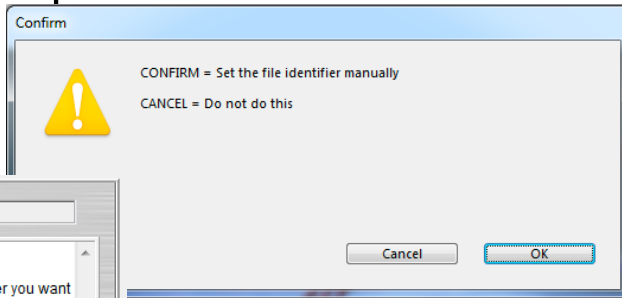


Set Graph Limit

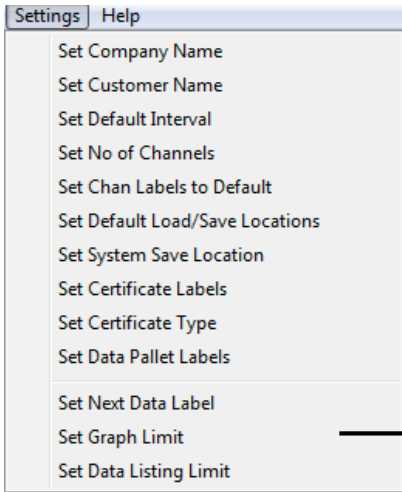


This sets the acquisition graph limit. This is a system limit set to prevent the processor becoming overloaded while graphing and acquiring. It sets the number of events showing in the acquisition graph before the graph starts to scroll out of the graphing display. Data acquired is not affected in any way.

A warning is presented here as this can affect the visual performance of the SDAS unit.

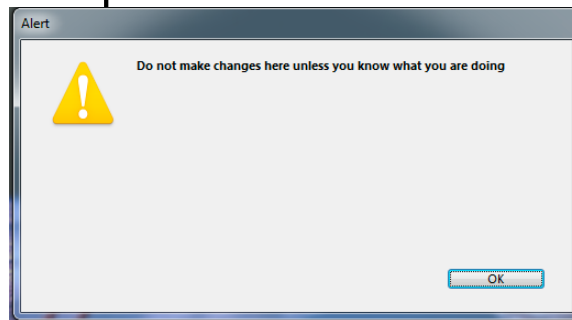

This is the number of points that are shown in the current acquiring graph before the graph starts to scroll right. You should not start resetting this unless you really need to see more current data points and are prepared to have an occasional display glitch if the processor gets busy. This does not affect the ability of the SDAS to collect and store data.

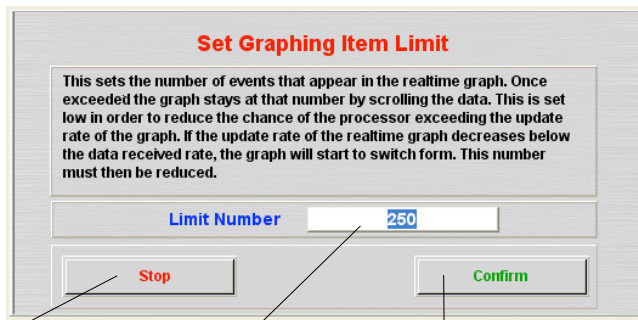


This leaves the setting unchanged

Enter the new value here

This confirms the change


Set Data Listing Limit

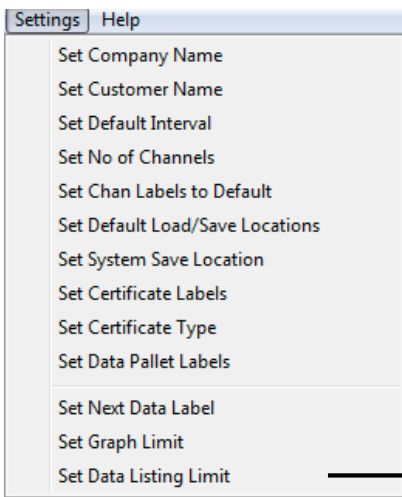

This sets the limit for acquired data listing. The option to show all data is disabled after this number of records and you are shown the data in smaller sections.

Sorting data and other actions like scrolling a list with more than this number can cause memory problems. If you have a need to operate with lists of more than this you can increase this number but be aware that you may experience core memory error messages which are quite blunt and in some cases the system may quit.

This is set to 100,000 by default

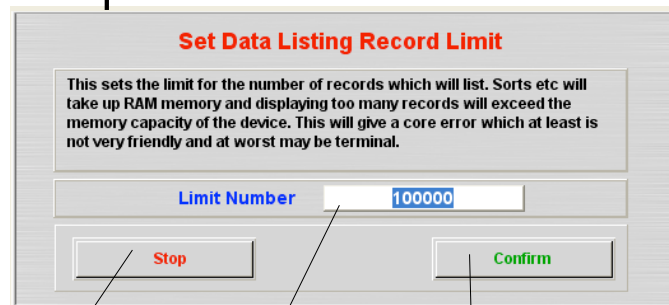

This leaves the setting unchanged

Enter the new value here


This confirms the change

Other SDAS Devices

Starting the SDAS program on a PC

The SDAS system can be run from a USB stick or a SDAS-6 program downloaded to a PC or PC laptop. This is then used to read from the stand alone range of scotia loggers. These loggers are set up and log using their own controls. The gathered data is then downloaded after the tests are complete. The downloading of the Scotialogger3, Scotialogger4 and SUDS devices are described here.

The folder containing the SDAS-6 must be found on the PC or USB stick. The folder will be labelled SDAS601.PC where the 601 will vary with the version of the current SDAS-6 program in use. Open this folder and identify the item SDAS.exe. Double click on it to launch the program. It should open full screen on the PC.

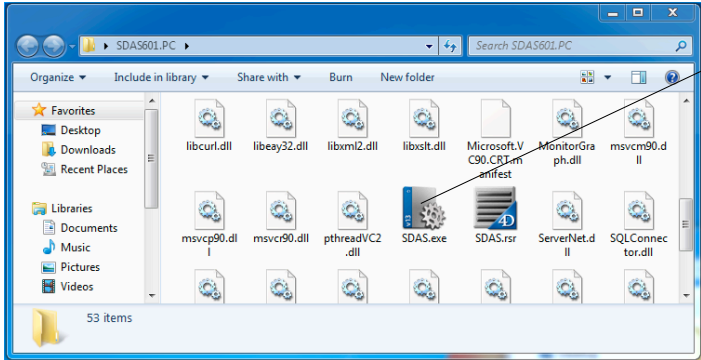

Launch this item to start the SDAS-6 program

When launched this screen appears on the PC




Scotialogger3

The Scotialogger3 device is a ruggedised single 4-20mA and 2 temperature device. When the data is gathered by the device it is stored in files which are displayed to the SDAS-6 software for downloading. The user can download as many files as they require. Note that the SDAS-6 program supplied with a ScotiaLogger3 may be matched to the device. If the software is linked to the logger's serial number then you cannot proceed to retrieve the data.


Select from the menus along the top of the screen.

Start Acquiring Data

This is the routine that acquires data into the SDAS-6 program. The ScotiaLogger3 should be connected to the PC or PC laptop and be switched on before starting this routine.

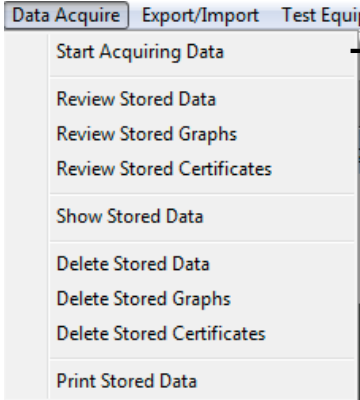


This screen appears showing the choice of files to download within the logger

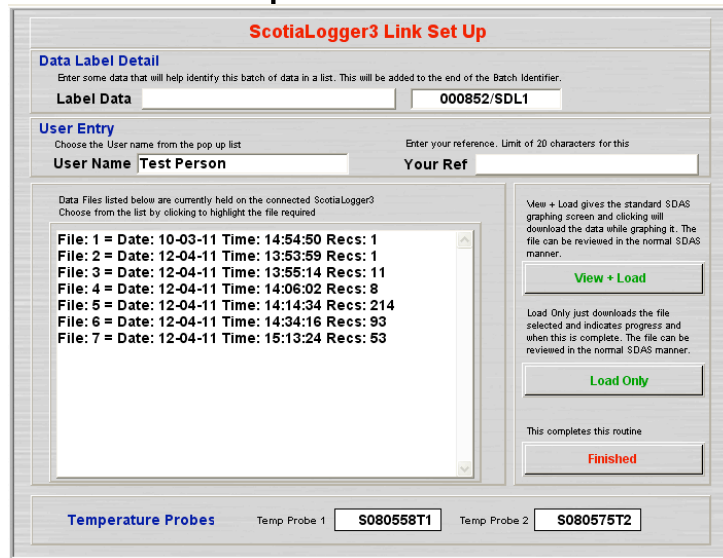

Enter the Label to be used for this file download

Enter the user reference to be used for this file download

Select the file to load by clicking on it to highlight it

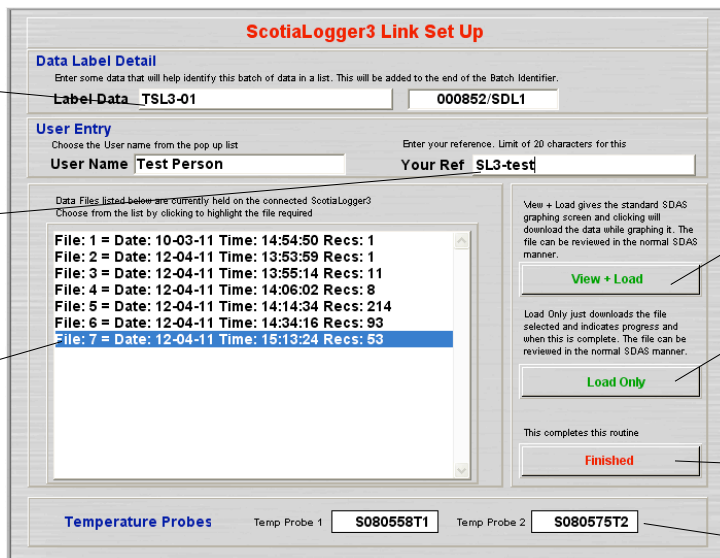

Click View + Load to select the file to load and open the logging screen

Click Load Only to select the file to load the file into the SDAS-6 database without viewing the download process.

Finished completes this routine

The serial number of the probes are loaded from the equipment file in the SDAS-6 program database as stored in Temp Probe 1 and Temp Probe 2. They are not loaded from the ScotiaLogger3. These should correspond to the probes used in those locations in the ScotiaLogger3. The user must ensure this is done.


When View + Load is clicked the following screen appears

Click Start Acq to start the import of the data from the chosen file in the ScotiaLogger3

The data is labelled as set in the previous screen by the user and the file number is added to the end in [07] brackets


The range is set by the ScotiaLogger3 data being imported

Since the ScotiaLogger3 only has one 4-20mA input only one channel is active

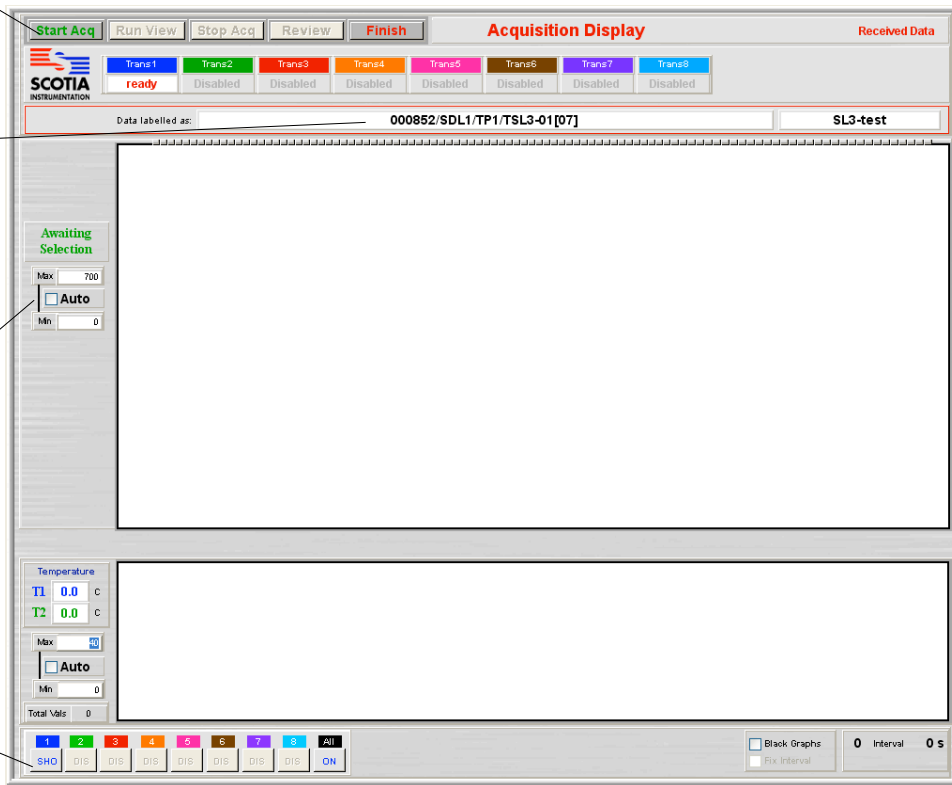

The file is then imported and shows graphing as it arrives. Importing stops at the end of the chosen file. The data is now saved in the SDAS-6 database

Review operates as the Review button in the normal SDAS-6

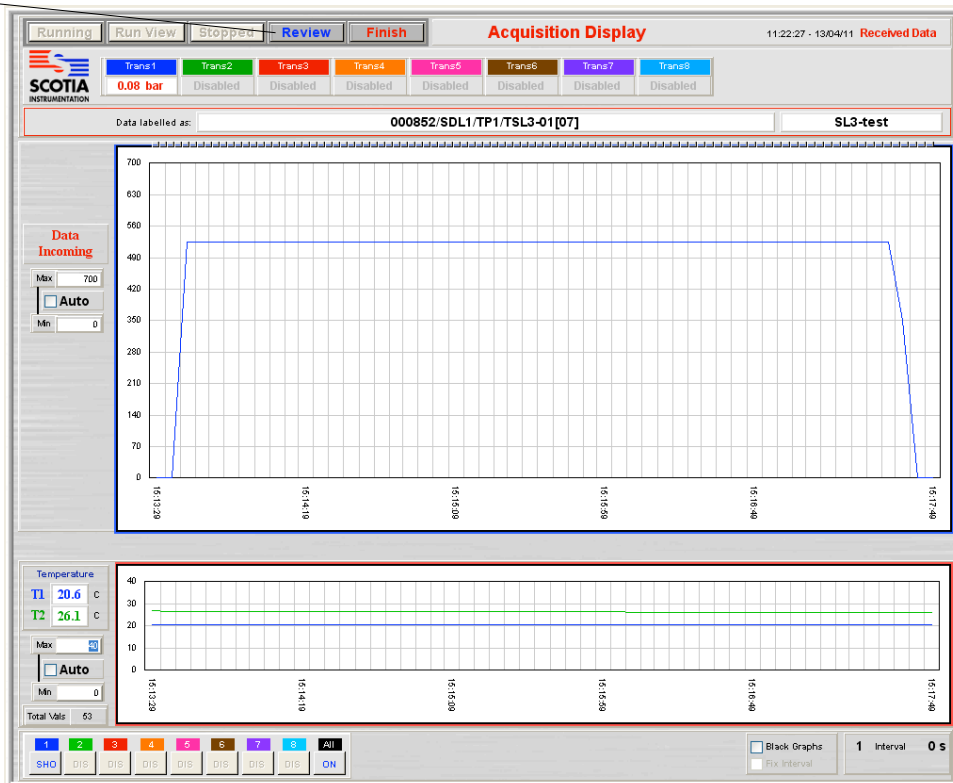

Clicking Finish returns to the import screen to allow another file to be imported. Enter the Label and reference data and select another file for importing or click Finished to end this routine.

ScotiaLogger3 Link Set Up

Data Label Detail
Enter some data that will help identify this batch of data in a list. This will be added to the end of the Batch Identifier.

Label Data

User Entry
Choose the User name from the pop up list Enter your reference. Limit of 20 characters for this

User Name Your Ref

Data Files listed below are currently held on the connected ScotiaLogger3
Choose from the list by clicking to highlight the file required

File: 1 = Date: 10-03-11 Time: 14:54:50 Recs: 1
File: 2 = Date: 12-04-11 Time: 13:53:59 Recs: 1
File: 3 = Date: 12-04-11 Time: 13:55:14 Recs: 11
File: 4 = Date: 12-04-11 Time: 14:06:02 Recs: 8
File: 5 = Date: 12-04-11 Time: 14:14:34 Recs: 214
File: 6 = Date: 12-04-11 Time: 14:34:16 Recs: 93
File: 7 = Date: 12-04-11 Time: 15:13:24 Recs: 53

View + Load gives the standard SDAS graphing screen and clicking will download the data while graphing it. The file can be reviewed in the normal SDAS manner.

View + Load

Load Only just downloads the file selected and indicates progress and when this is complete. The file can be reviewed in the normal SDAS manner.

Load Only

This completes this routine

Finished

Temperature Probes Temp Probe 1 Temp Probe 2

Finished completes this routine


SUDS

The Scotia Underwater Datalogger System (SUDS) device is a logger system designed to operate at low power and be housed in a subsea enclosure pod although it can be deployed elsewhere. It can have five 4-20mA inputs, 1 pt-100 temperature input and 3 flow inputs. When the data is gathered by the device it is stored in files which are displayed to the SDAS-6 software for downloading. The user can download as many files as they require. Note that the SDAS-6 program supplied with a SUDS is matched to the device. If the SUDS serial number does not match that stored in the SDAS-6 program then you cannot proceed to gather data. The transmitters used by the SUDS must also be included in the equipment data file of the SDAS-6 program otherwise the SDAS-6 Review system cannot determine the range of transmitters. Failure to do this will result in warnings that the ranges may be incorrect.



Select from the menus along the top of the screen.

Start Acquiring Data

This is the routine that acquires data into the SDAS-6 program. The SUDS should be connected to the PC or PC laptop and be switched on before starting this routine.

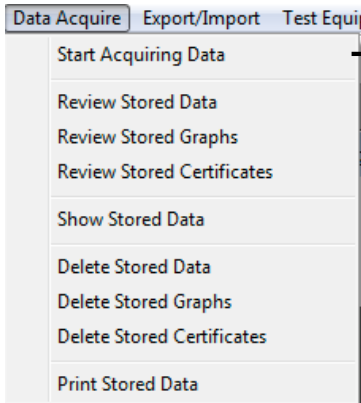

This screen appears showing the choice of files within the SUDS

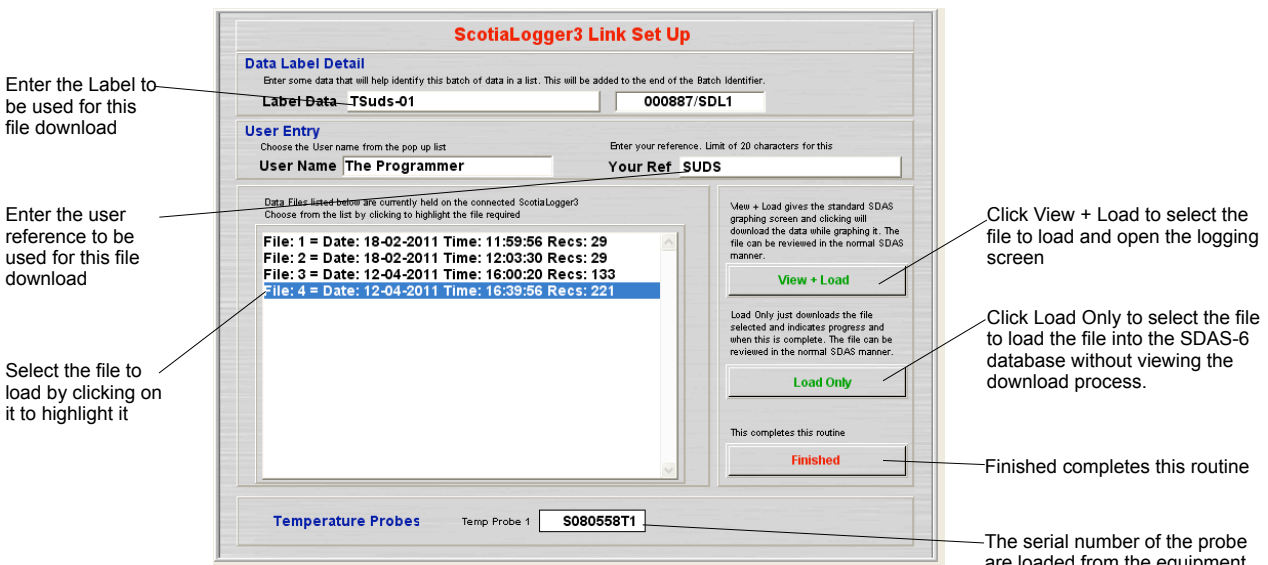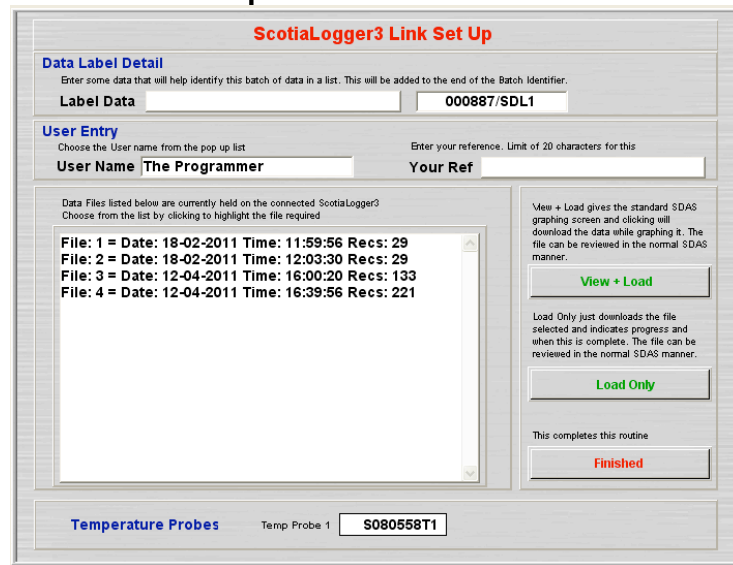


When View + Load is clicked the following screen appears

Click Start Acq to start the import of the data from the chosen file in the SUDS

The data is labelled as set in the previous screen by the user and the file number is added to the end in [07] brackets

The range is set by the SUDS data being imported


This shows the SUDS active channels

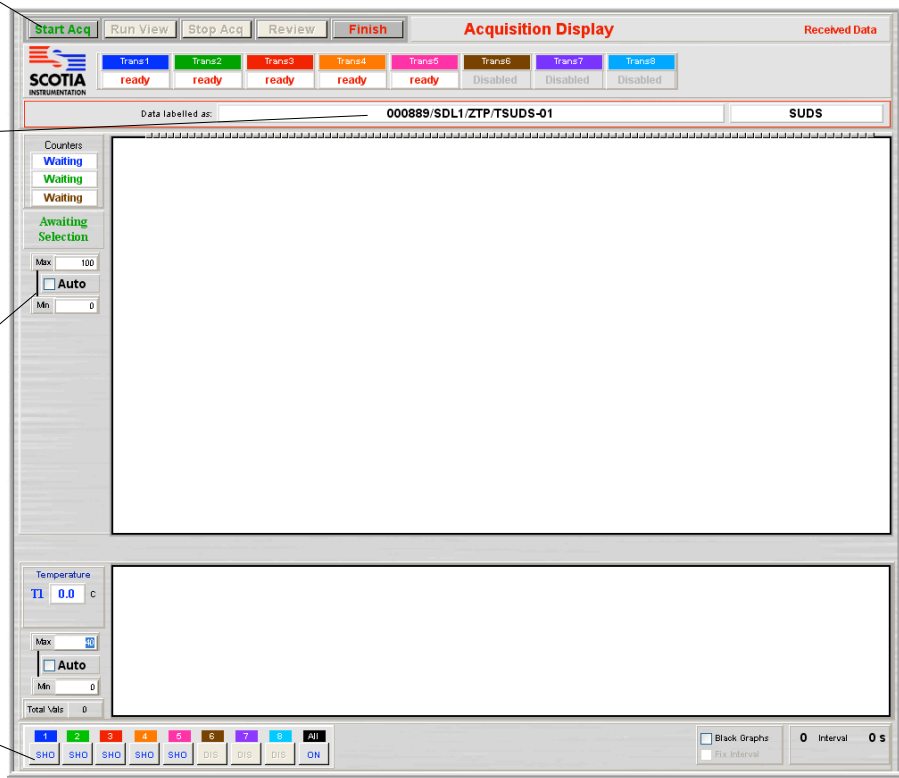

The file is then imported and shows graphing as it arrives. Importing stops at the end of the chosen file. The data is now saved in the SDAS-6 database

Review operates as the Review button in the normal SDAS-6

In this case the units of the graphed values are not all the same so the 0-100% scale shows

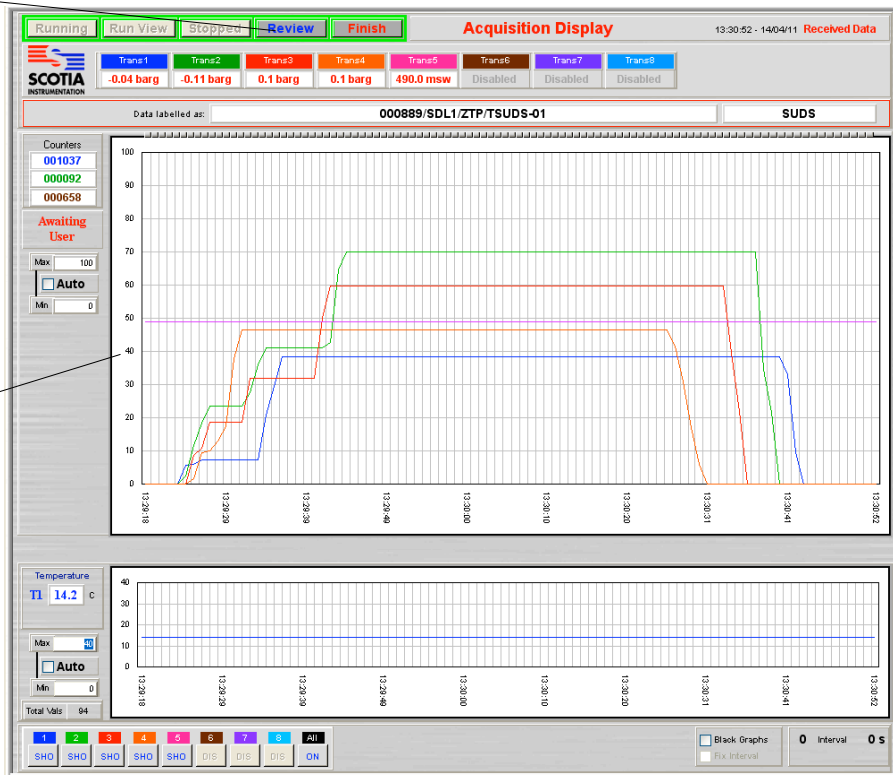

Clicking Finish returns to the import screen to allow another file to be imported. Enter the Label and reference data and select another file for importing or click Finished to end this routine.

ScotiaLogger3 Link Set Up

Data Label Detail
Enter some data that will help identify this batch of data in a list. This will be added to the end of the Batch Identifier.
Label Data

User Entry
Choose the User name from the pop up list Enter your reference. Limit of 20 characters for this
User Name Your Ref

Data Files listed below are currently held on the connected ScotiaLogger3
Choose from the list by clicking to highlight the file required

File: 1 = Date: 18-02-2011 Time: 11:59:56 Recs: 29
File: 2 = Date: 18-02-2011 Time: 12:03:30 Recs: 29
File: 3 = Date: 12-04-2011 Time: 16:00:20 Recs: 133
File: 4 = Date: 12-04-2011 Time: 16:39:56 Recs: 221

View + Load gives the standard SDAS graphing screen and clicking will download the data while graphing it. The file can be reviewed in the normal SDAS manner.

View + Load

Load Only just downloads the file selected and indicates progress and when this is complete. The file can be reviewed in the normal SDAS manner.

Load Only

This completes this routine

Finished

Temperature Probes Temp Probe 1

Finished completes this routine

SDAS Options

The SDAS system can have various options added to meet customer requirements. The following are the available options at version 6.07. If you have a requirement which is not met by the list of standard options then please discuss this with the technical or sales department at Scotia and we will consider adding your requirements to either a special version or adding an additional option.

Counter Options

This adds a counter option to the SDAS.

The SDAS5 can currently have up to three counters fitted. Counters 1 and 3 have no debounce electronic circuitry and so cannot be used to read the switching of a stroke counter mechanical switch. They are designed to work with an inductive sensor used with items such as a mechanical flow meter. Counter 2 has debounce circuitry to enable it to work with a mechanical counter. It is optimised for this and as such cannot accept fast switching.

The following screens show all three counters active. If any are not active then they do not appear on these screens.

Data Acquisition Set Up

Select channels for scale setting or enabling/disabling by clicking here

Common Ch1 = ON Ch2 = ON Ch3 = ON Ch4 = ON Ch5 = ON Ch6 = ON Ch7 = ON Ch8 = ON

Data Label Detail
Enter some data that will help identify this batch of data in a list of saved files. There is an 80 character limit for this entry
Label Data TSC004
The above will be added to the end of the Batch Identifier shown here: 000812/S088223 Add to saved data

User Entry
Currently logged in system user: Review Person
Enter your reference. Limit of 20 characters for this: CT001

Acquisition events rate (seconds) 0 Skip Tare Routine

Set Graph Scale
The graphs will scale to match the pressure and temperature data if the Auto box is checked below. If unchecked the scale limits are set in the boxes shown. This can also be toggled on the graph screen. The screen label for each channel can be set below.

Channel Labels	Trans1	Trans2	Trans3	Trans4	Trans5	Trans6	Trans7	Trans8	Temperature
Min	0	0	0	0	0	0	0	0	0
Max	700	800	1000	1000	1300	1300	1500	1500	40
Unit	barg	barg	barg	barg	barg	barg	barg	barg	C

Temperature Probes
Temp Probe 1: S080558T1 Temp Probe 2: S080558T2 Probe 2 Off

Counter Readings
Current Counter Values: 0 0 0

Stop Proceed

With this active the counter section is shown. The counters are zeroed for starting. They appear here for confirmation.

The zero offset screen then appears

Zero Offset Transmitters

Data Label: 000812/S088223/RP1/TSC004


Transmitter	Channel	Range	Min	Max	Unit
Trans1	S080558ch1	Range	0	700	barg
Trans2	S080558ch2	Range	0	800	barg
Trans3	S080558ch3	Range	0	1000	barg
Trans4	S080558ch4	Range	0	1000	barg
Trans5	S080558ch5	Range	0	1300	barg
Trans6	S080558ch6	Range	0	1300	barg
Trans7	S080558ch7	Range	0	1500	barg
Trans8	S080558ch8	Range	0	1500	barg

Transmitter 1 Currently Reads	-0.168	Offset this to the 0 barg value	<input checked="" type="checkbox"/> Set
Transmitter 2 Currently Reads	-0.112	Offset this to the 0 barg value	<input checked="" type="checkbox"/> Set
Transmitter 3 Currently Reads	0.24667	Offset this to the 0 barg value	<input checked="" type="checkbox"/> Set
Transmitter 4 Currently Reads	0.97	Offset this to the 0 barg value	<input checked="" type="checkbox"/> Set
Transmitter 5 Currently Reads	0.64567	Offset this to the 0 barg value	<input checked="" type="checkbox"/> Set
Transmitter 6 Currently Reads	0.32067	Offset this to the 0 barg value	<input checked="" type="checkbox"/> Set
Transmitter 7 Currently Reads	0.425	Offset this to the 0 barg value	<input checked="" type="checkbox"/> Set
Transmitter 8 Currently Reads	-0.005	Offset this to the 0 barg value	<input checked="" type="checkbox"/> Set

Transmitter values shown in red exceed the recommended amount for offsetting. Those in green may have non-zero values.

Do not Offset Apply Offset


When the Acquisition screen appears the counters appear here and show as Waiting

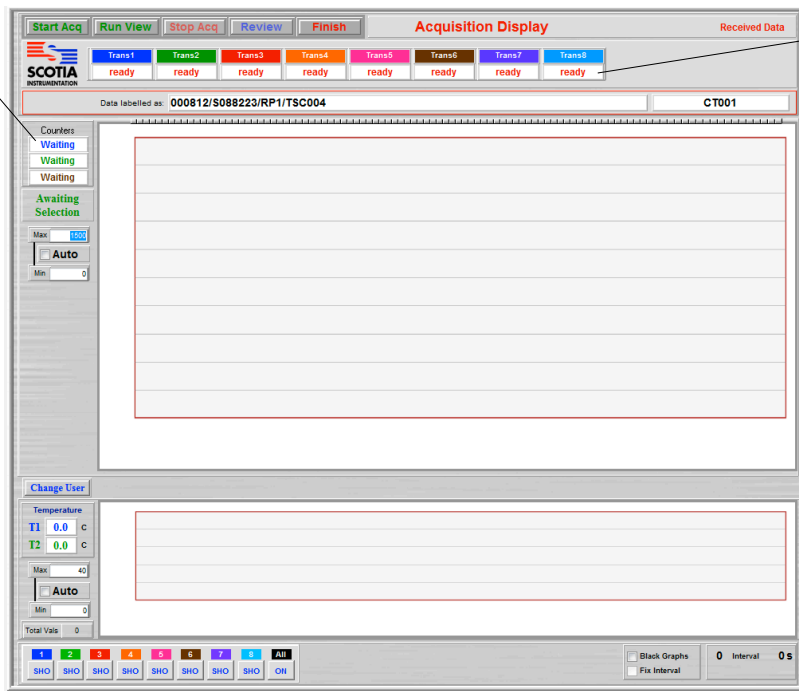

The transmitter readings show as ready

No data has been received from the temperature probes


When Acquisition starts the counters appear here and the values update every second regardless of the logging interval. The values are only logged at the set interval.

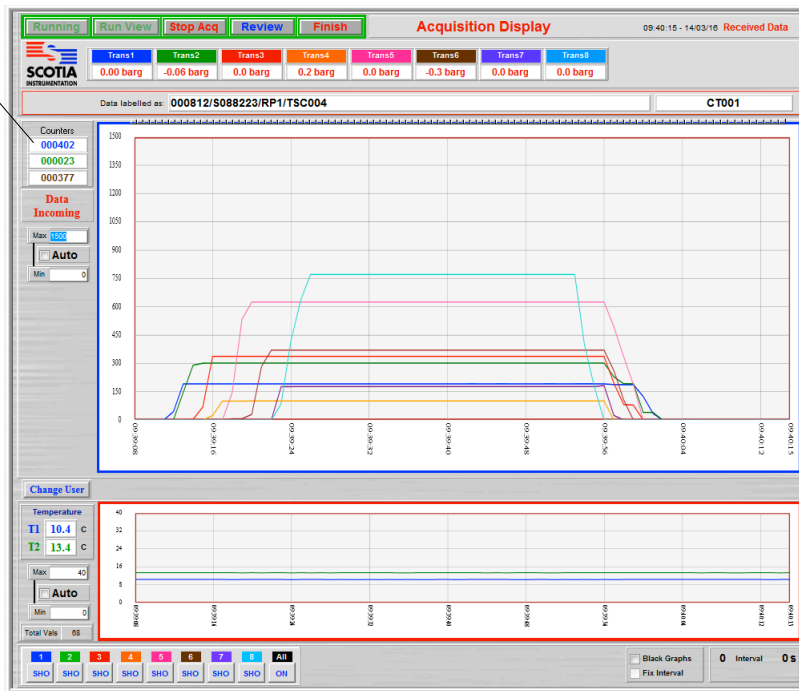

Clicking Review leads to the following screen


In Review the counters appear here.

Note that in Review the counters show the count difference between the left side value and Location Marker. Zero is shown initially as the Location Marker is placed far left. When the Location Marker is placed elsewhere the counters update to show the count difference to that point.

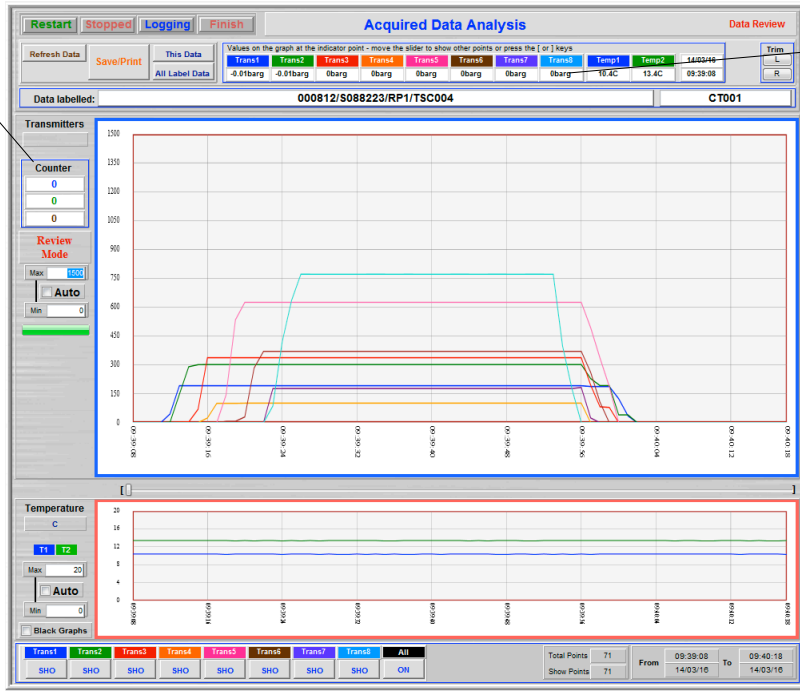

The transmitter values at the Location Marker are shown. The Location Marker is placed on the left side of the graph when the screen appears so these values are the readings on the left of the graph


The counters now show the difference in counts between the left of the graph and the Location Marker

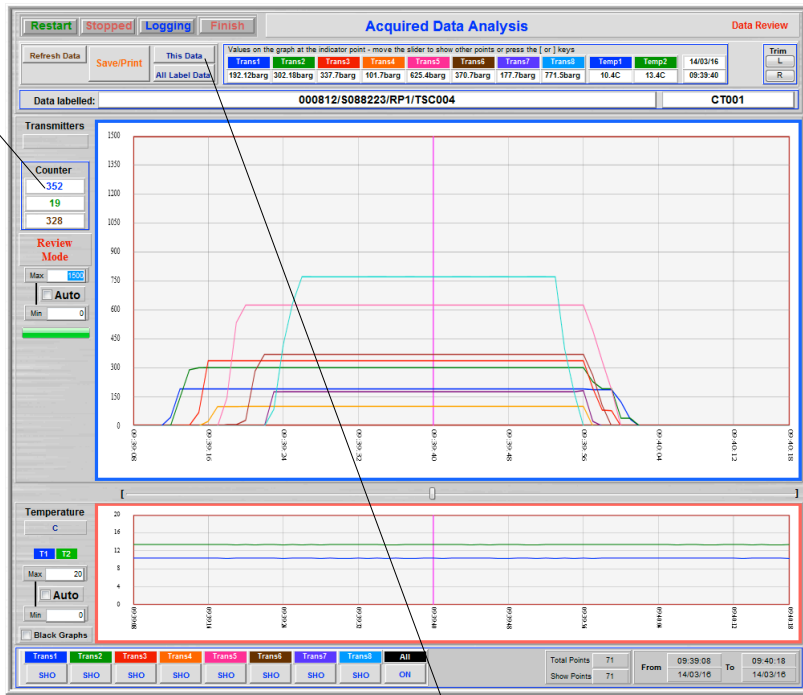

Clicking This Data allows the user to examine the data and perhaps select the data point where the counters stop. Clicking on that value will set the left graph point. Clicking again will set the right data point if necessary. Another click repeats this.


Item	Time	Date	Trans 1	Trans 2	Trans 3	Trans 4	Trans 5	Trans 6	Trans 7	Trans 8	Counter 1	Counter 2	Counter 3	Temp 1	Temp 2
1567100	09:39:35	14/03/16	192.11	302.19	337.7	101.7	625.4	370.7	177.7	771.5	331	19	312	10.30	13.30
1567101	09:39:38	14/03/16	192.11	302.14	337.7	101.7	625.4	370.7	177.6	771.4	343	20	319	10.40	13.30
1567102	09:39:37	14/03/16	192.11	302.17	337.7	101.7	625.4	370.7	177.6	771.5	351	20	327	10.30	13.40
1567103	09:39:38	14/03/16	192.12	302.17	337.7	101.7	625.5	370.7	177.7	771.5	367	21	342	10.30	13.40
1567104	09:39:38	14/03/16	192.11	302.15	337.7	101.7	625.4	370.7	177.6	771.4	375	21	349	10.40	13.40
1567105	09:39:40	14/03/16	192.12	302.18	337.7	101.7	625.4	370.7	177.7	771.5	391	22	364	10.40	13.40
1567106	09:39:41	14/03/16	192.1	302.19	337.7	101.7	625.4	370.7	177.6	771.4	399	23	371	10.30	13.40
1567107	09:39:40	14/03/16	192.10	302.15	337.7	101.7	625.4	370.7	177.6	771.5	402	23	372	10.30	13.30
1567108	09:39:43	14/03/16	192.12	302.15	337.7	101.7	625.4	370.7	177.6	771.5	402	23	377	10.40	13.40
1567109	09:39:44	14/03/16	192.11	302.15	337.7	101.7	625.5	370.7	177.7	771.5	402	23	377	10.40	13.30
1567110	09:39:46	14/03/16	192.12	302.17	337.7	101.7	625.4	370.7	177.6	771.4	402	23	377	10.40	13.40
1567111	09:39:46	14/03/16	192.12	302.15	337.7	101.7	625.4	370.7	177.6	771.5	402	23	377	10.40	13.30
1567112	09:39:47	14/03/16	192.11	302.17	337.7	101.7	625.4	370.7	177.6	771.5	402	23	377	10.30	13.40
1567113	09:39:48	14/03/16	192.11	302.18	337.7	101.7	625.5	370.7	177.7	771.5	402	23	377	10.30	13.40
1567114	09:39:49	14/03/16	192.11	302.17	337.7	101.7	625.4	370.7	177.6	771.4	402	23	377	10.40	13.40
1567115	09:39:49	14/03/16	192.10	302.17	337.7	101.7	625.4	370.7	177.7	771.5	403	23	377	10.40	13.30

Clicking Regraph shows this screen

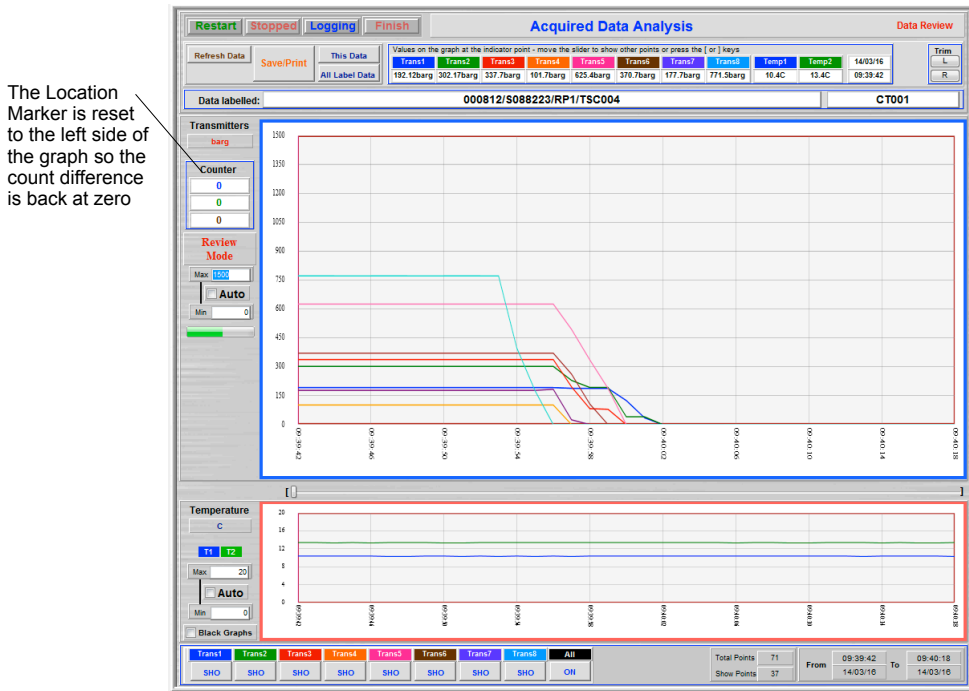

The Location Marker is reset to the left side of the graph so the count difference is back at zero

Clicking Save/Print before altering the graph above leads to the following screen

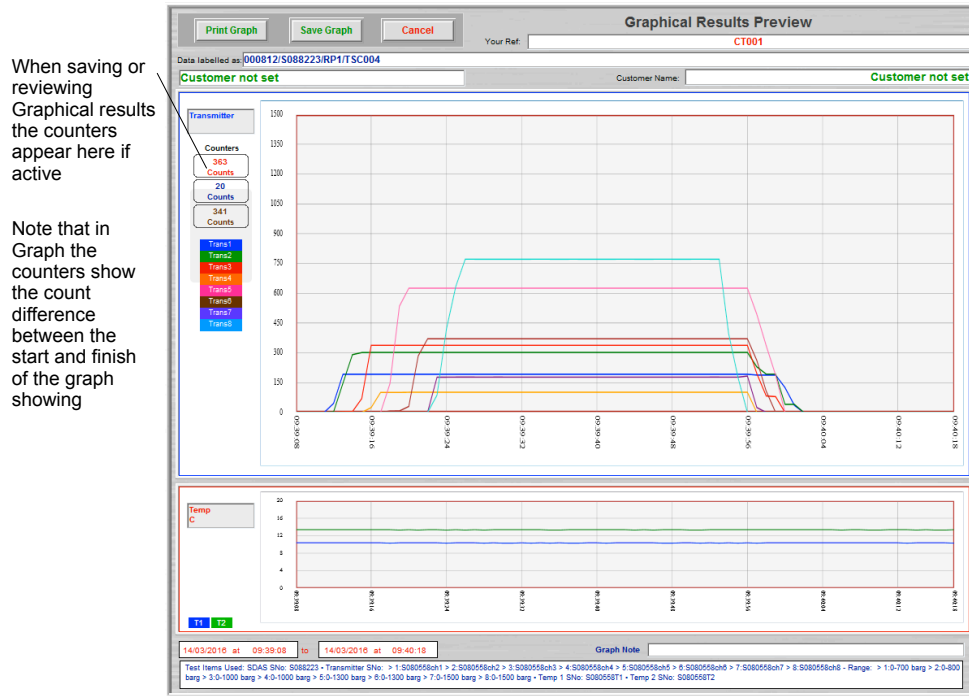

When saving or reviewing Graphical results the counters appear here if active

Note that in Graph the counters show the count difference between the start and finish of the graph showing

Clicking Print Graph will save and print the detail shown

Clicking Save Graph just saves the graph to the data file

Clicking Cancel returns to the previous screen making no changes

Variable Data Rate Option

This allows the user to set the rate at which data is saved to the data file at the start and then change this rate while gathering data. Note that the data will update on screen every second but will be saved to the data file at the rate set. It should also be noted that the time line shows data events and does not alter if you change the time between events. This can be misleading if the user reads the graph time line as linear. The time line is marked correctly and all the data is time and date marked correctly.




When this option is active the Set value can be changed by clicking on the item and typing a new value in. Note that the entry is live and the rate of data gathering will act on the new value as you type it in.


Hold Period Timer Option

This is a stopwatch type option which allows the user to time any event in a countdown mode. The user sets the period of countdown at the start of the acquisition sequence. At any time the countdown can be started. When the time has elapsed the timer shows 'Finish'. The timer can be reset at any time and the countdown restarted. When the data acquisition is stopped the timer countdown also pauses and restarts when the acquisition restarts.

This screen shows in the set up sequence before the logging screen appears

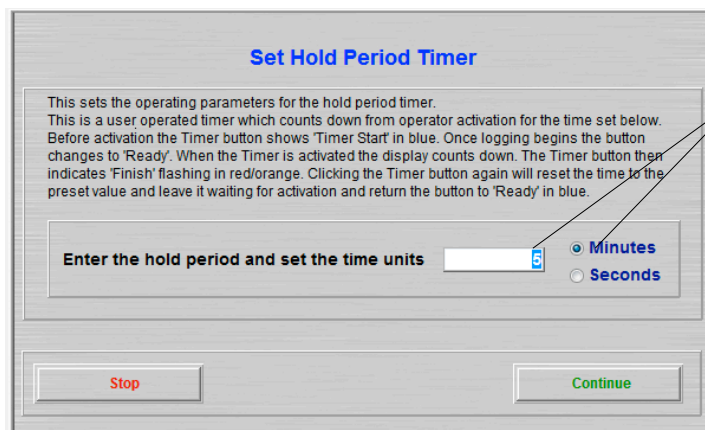


Enter the hold period in minutes or seconds and check the time units button

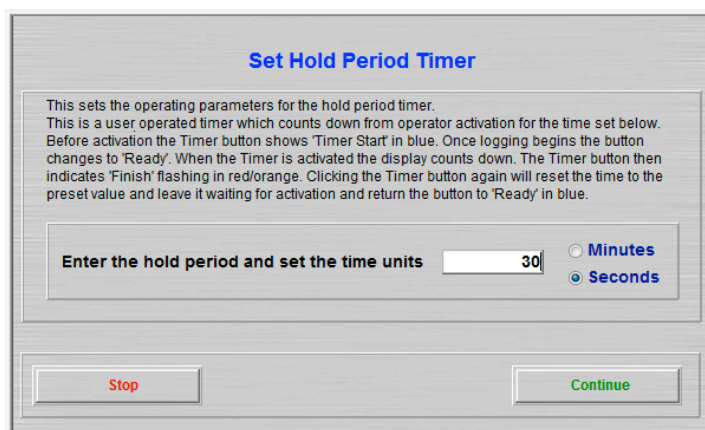


Setting to 30 seconds would look like this


With this option activated this button appears. Before logging starts it shows like this

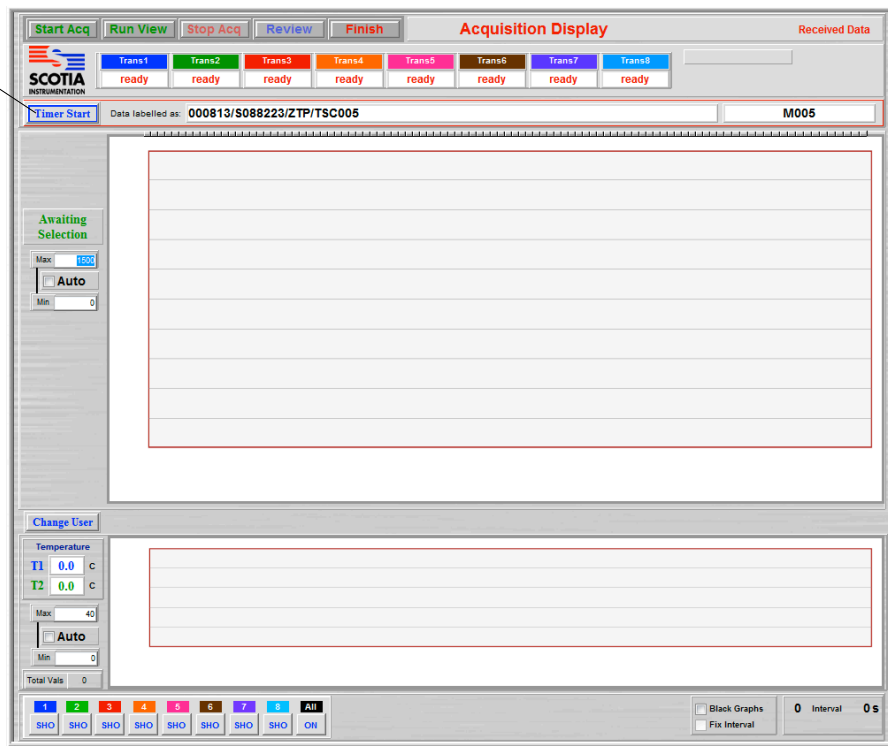


When data gathering starts the button changes to Ready




When the timer has been activated the button changes to counting down the time to the finish. If clicked again it then resets the Hold Timer



When the timer finishes counting down it changes to Finish and flashes red and orange




When clicked again the button resets the count to zero and changes to Ready




Test Event Log Option

This option allows the user to view events that have happened during a data acquisition. Most button actions and events are reported to this log. This can allow the period of the acquisition to be checked for any events which might compromise the continuity of the test.

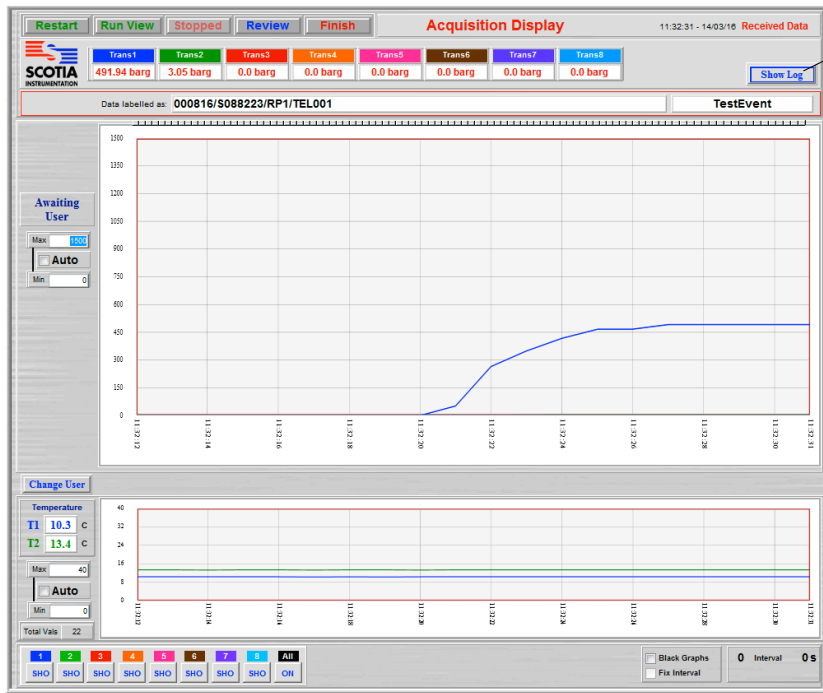



The Show Log shows when this option is active. Clicking this displays the event log screen.

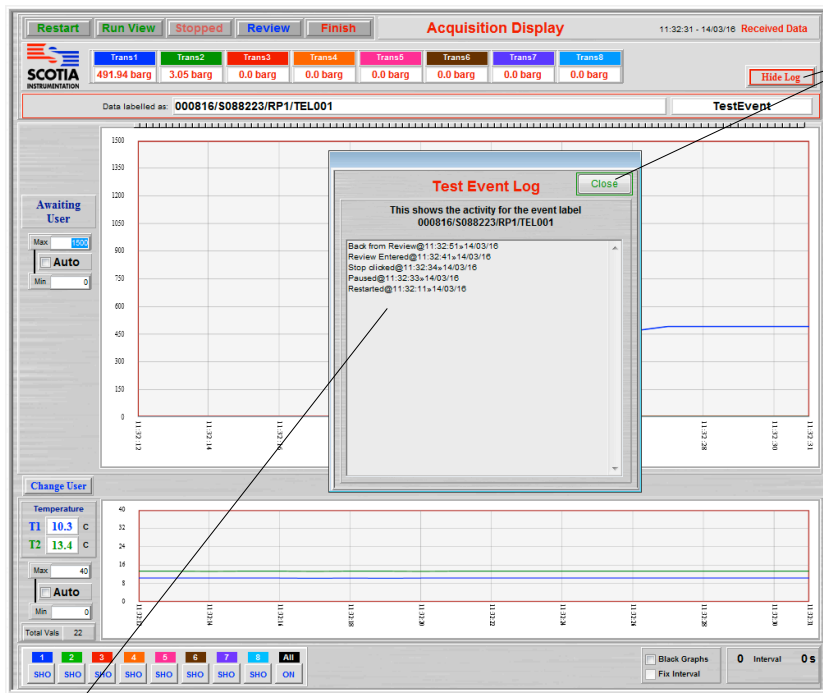

When activated the button changes to 'Hide Log'. Clicking this button again hides the Log screen. The Log Screen can also be closed by clicking the Close button

When this log screen is visible it is totally inert. It shows events but merely blocks the view of the screen under where it is sitting. The screen behind is still fully active. The data updates when logging is active. It can be moved about the screen by clicking on the top bar and holding the mouse down as it is dragged. Acquisition is not affected by the appearance of this screen. The Test Event Log screen is removed by clicking the Close button, clicking the Hide Log on the acquisition screen or closing the acquisition screen. Event data is added in time sequence to the top of the log file.

After acquisition has finished the event log can be seen from the Utilities menu - View System Log.

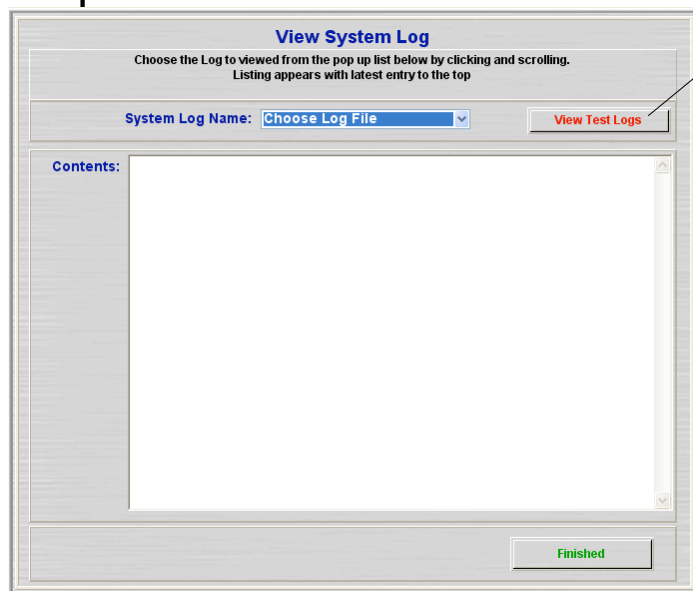

When this option is active this button appears on the View System Log screen. Clicking this button brings up a file selection screen as shown in the Utilities menu section of this manual.

Alarm Option

This option allows the user to set an alarm for each channel of the SDAS transmitter channels. The alarm is not only announced visually on screen but the SDAS unit also closes a relay with volt-free contacts. This can be connected to an external alarm system. Note that there is just one alarm switch and it will go into closed mode and stay closed while any of the alarms are active. Each of the alarms can be triggered in either rising or falling mode. In rising mode the alarm is triggered when the value of the transmitter rises above the set value. The alarm stays triggered until it is reset or the data acquisition is stopped. When in falling mode the alarm is armed when the value of the transmitter rises above the set value and then is triggered when the value drops below this value. Each alarm can be cancelled separately. If the acquisition is stopped then this cancels all alarm modes. Each alarm can be cancelled and reset separately.

Set Alarm Parameters

This sets the operating parameters for alarm activation.
Set the alarm value in the units of the transmitter.
The alarm trips at the set point, flashes the reset button and closes the alarm contacts on the unit.
Once tripped the alarm can be cancelled by clicking the alarm button.
Each alarm can be reset but must sense the alarm condition to trip again.
The alarm can be tripped either rising or falling.
Alarm set points MUST be in the same units as the transmitter acquired data.

Channel	Alarm on	Alarm Point	Mode
Alarm Channel 1	<input type="checkbox"/>	Enter the alarm point	<input type="radio"/> Rising <input type="radio"/> Falling
Alarm Channel 2	<input type="checkbox"/>	0	<input type="radio"/> Rising <input checked="" type="radio"/> Falling
Alarm Channel 3	<input type="checkbox"/>	0	<input type="radio"/> Rising <input checked="" type="radio"/> Falling
Alarm Channel 4	<input type="checkbox"/>	0	<input type="radio"/> Rising <input checked="" type="radio"/> Falling
Alarm Channel 5	<input type="checkbox"/>	0	<input type="radio"/> Rising <input checked="" type="radio"/> Falling
Alarm Channel 6	<input type="checkbox"/>	0	<input type="radio"/> Rising <input checked="" type="radio"/> Falling
Alarm Channel 7	<input type="checkbox"/>	0	<input type="radio"/> Rising <input checked="" type="radio"/> Falling
Alarm Channel 8	<input type="checkbox"/>	0	<input type="radio"/> Rising <input checked="" type="radio"/> Falling

Buttons: Leave Alarms Unset, Set Selected Alarms

Callouts:
 - Check or uncheck these to turn each alarm on or off (points to 'Alarm on' checkboxes)
 - The alarm value is entered here but is only active if the Alarm On box is checked. Enter each active alarm's value in the units of the transmitter used. (points to 'Enter the alarm point' field)
 - Toggle these to select rising or falling alarm (points to mode radio buttons)

In this case alarms for channels 1 2 and 6 are set and alarms for 3 4 5 7 and 8 are not set


Set Alarm Parameters

This sets the operating parameters for alarm activation.
Set the alarm value in the units of the transmitter.
The alarm trips at the set point, flashes the reset button and closes the alarm contacts on the unit.
Once tripped the alarm can be cancelled by clicking the alarm button.
Each alarm can be reset but must sense the alarm condition to trip again.
The alarm can be tripped either rising or falling.
Alarm set points MUST be in the same units as the transmitter acquired data.


Channel	Alarm on	Alarm Point	Mode
Alarm Channel 1	<input checked="" type="checkbox"/>	300	<input type="radio"/> Rising <input checked="" type="radio"/> Falling
Alarm Channel 2	<input checked="" type="checkbox"/>	500	<input type="radio"/> Rising <input checked="" type="radio"/> Falling
Alarm Channel 3	<input type="checkbox"/>	0	<input type="radio"/> Rising <input checked="" type="radio"/> Falling
Alarm Channel 4	<input type="checkbox"/>	0	<input type="radio"/> Rising <input checked="" type="radio"/> Falling
Alarm Channel 5	<input type="checkbox"/>	0	<input type="radio"/> Rising <input checked="" type="radio"/> Falling
Alarm Channel 6	<input checked="" type="checkbox"/>	750	<input type="radio"/> Rising <input checked="" type="radio"/> Falling
Alarm Channel 7	<input type="checkbox"/>	0	<input type="radio"/> Rising <input checked="" type="radio"/> Falling
Alarm Channel 8	<input type="checkbox"/>	0	<input type="radio"/> Rising <input checked="" type="radio"/> Falling

Buttons: Leave Alarms Unset, Set Selected Alarms


Callouts:
 - This proceeds with all the alarms unset (points to 'Leave Alarms Unset' button)
 - This confirms the alarms as set (points to 'Set Selected Alarms' button)

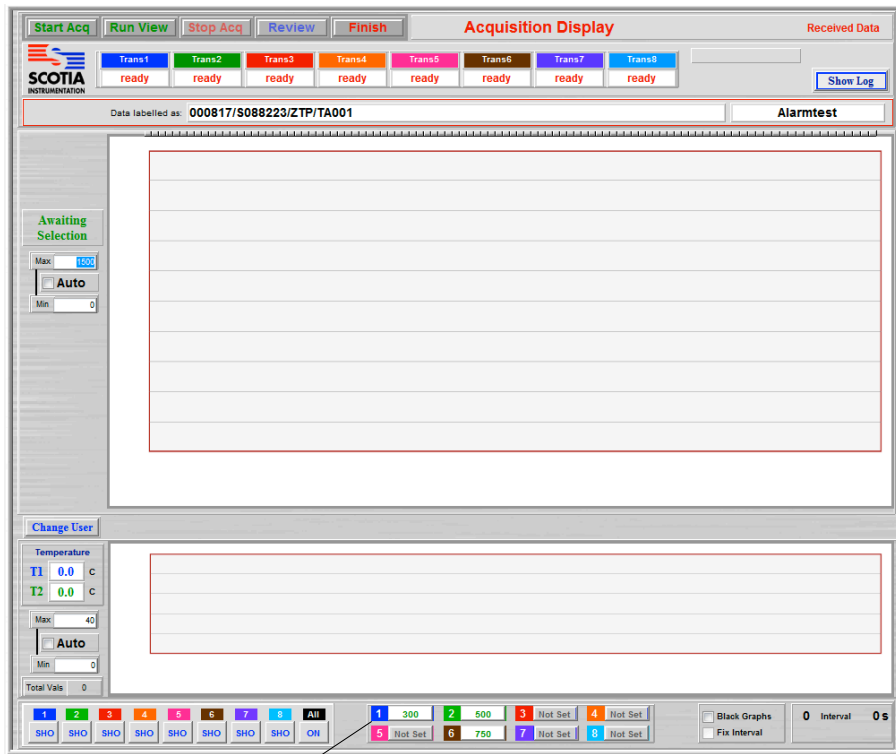

When the acquisition starts the state of the alarms for each channel are shown here numbered and colour coded to the channel graph. Those set have their set value indicated in green. Those not set have 'Not Set' showing and are disabled.

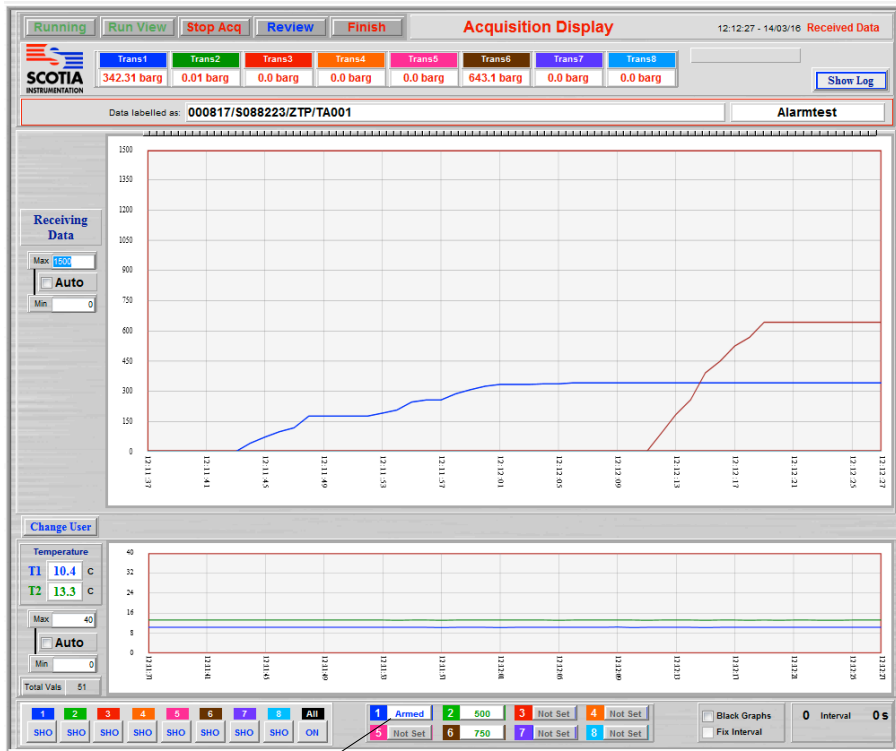

If the alarm is set for Falling Alarm the indication changes to Armed and the set value in blue flashing alternately. If the data acquisition is stopped this setting is held waiting for acquisition to restart. If the button is clicked then this cancels the alarm arming and it changes to Set Off. Clicking it again resets alarm to its initial state allowing it to be triggered again. Note that a falling alarm needs to pass rising through the trigger point for the alarm to become active.

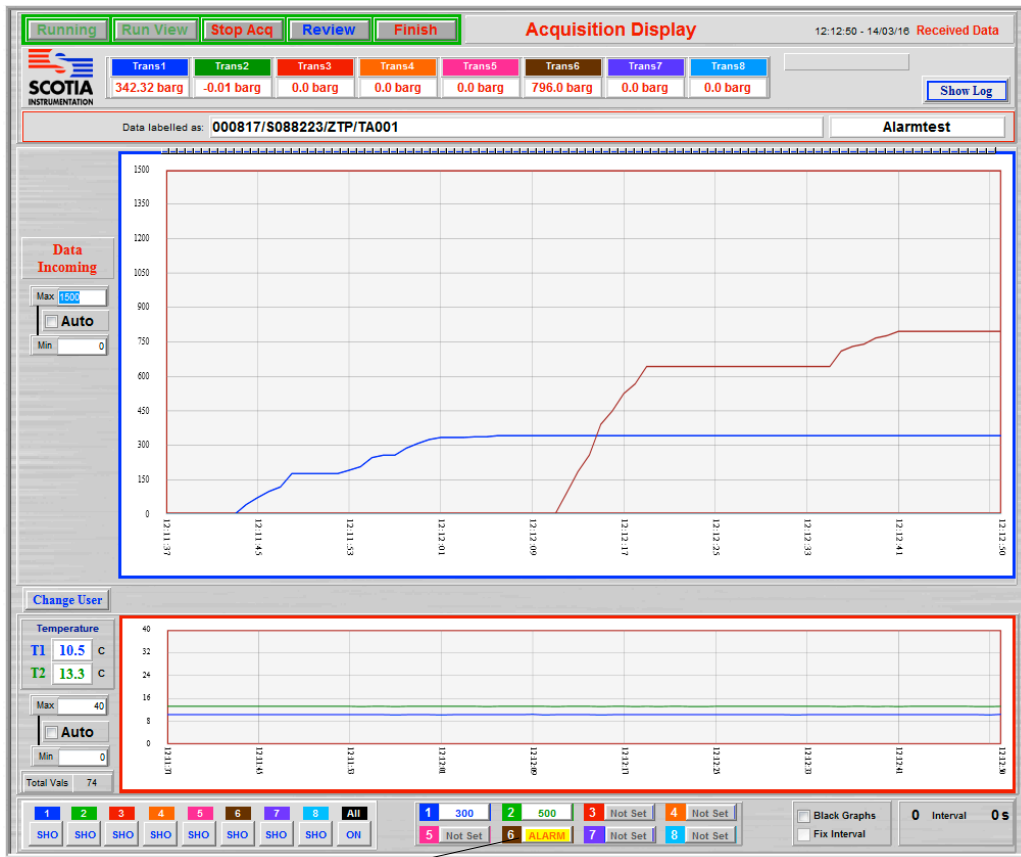

Channel 6 is now in alarm and shows ALARM ACTIVE alternately in red on yellow. The SDAS also activates its internal alarm switch which can be wired to an audible or visual externally powered system.



More than one alarm can be active at once - although only one external alarm can be connected. The alarm switch is held active until all the alarms are cancelled.



If an alarm button is clicked when in alarm it goes to Set Off. When clicked at Set Off it then resets to Reset if acquisition is currently stopped and the set point in green if the acquisition is running. If clicked again it changes to Set Off. When at Reset it changes to the set point in green when acquisition restarts.

When acquisition stops any active alarms are set to Set Off and the internal alarm switch sets to off.

Certificates Option

Set Certificate Labels

Settings Help

- Set Company Name
- Set Customer Name
- Set Default Interval
- Set No of Channels
- Set Chan Labels to Default
- Set Default Load/Save Locations
- Set System Save Location
- Set Certificate Labels
- Set Certificate Type
- Set Data Pallet Labels
- Set Next Data Label
- Set Graph Limit
- Set Data Listing Limit

When this option is active it allows creating and printing a test certificate. The labels of the certificate can be set in the utilities menu initially and this needs to be set by the user before creating any certificates. Once set the detail is saved and can be exported for use by other SDAS units creating certificates.

Test Inspection Certificate Labels

This sets the labels for this test certificate - Enter or change the Label Details below

Certificate Title		Hydrostatic Test Inspection Certificate	
Issuing Company		Company Testing Centre Ltd	
Issuing Coy Address		CTC Place, Somewhere, Aberdeen	
Client			
Client Contract			
Client Job No			
CTC Reference			
SDAS Data Label			
Items Inspected			
Drawing No(s)			
Spool No(s)			
Location			
Test Type			
Test Pressure			
Test Medium			
Test Duration			
	Time	Date	Pressure
Test On			
Test Off			
SDAS Serial Number			
Pressure Transmitter			
Range			
Traceable Standard			
Pipewall Temperature Probe Serial No			

Each of the areas with a white background can be set to any typed entry. These labels appear in the certificate against data entered.

This gives a versatile certificate labeling system that will allow changes as the user requires within the constraints of the overall certificate system.

The labels are saved with the certificate so future changes to the labels will not be reflected in previously saved certificates.

Creating Certificates

When this option is active it allows creating and printing a test certificate. The labels of the certificate must be set in the utilities menu initially and this needs to be set by the user before creating any certificates. The labels are saved with each certificate so changing the labels for later certificates does not alter the saved form of previous certificates.


The certificates are linked to a test being performed using the SDAS. In order to utilise some of the data from the saved test the certificate creation is not called from a menu item but from within the Review of the test data.

To create a Certificate the user enters Review of the stored data either from the Review button on the Acquire routine or from Review Stored Data menu item. Choose the part of the graph area which represents the period of the test - e.g. the hold period - and then choose Save/Print.

Enter Review of Data - find your test and display all the test and then reduce the test period to the period over which you are issuing the test certificate using the trimming bar or the Data buttons. If it is a hold test then choose the start and finish of the hold period.


Note: Currently the certificate routine only works for Graphs with just one graph line. You must choose to show just one graph line before proceeding to save the Graph and the Certificate. Multi line graphs can be used but a certificate can only be produced for one line on a test. You MUST reduce the graph to the line and section of it that you wish to use before clicking Save/Print.

Data gathering

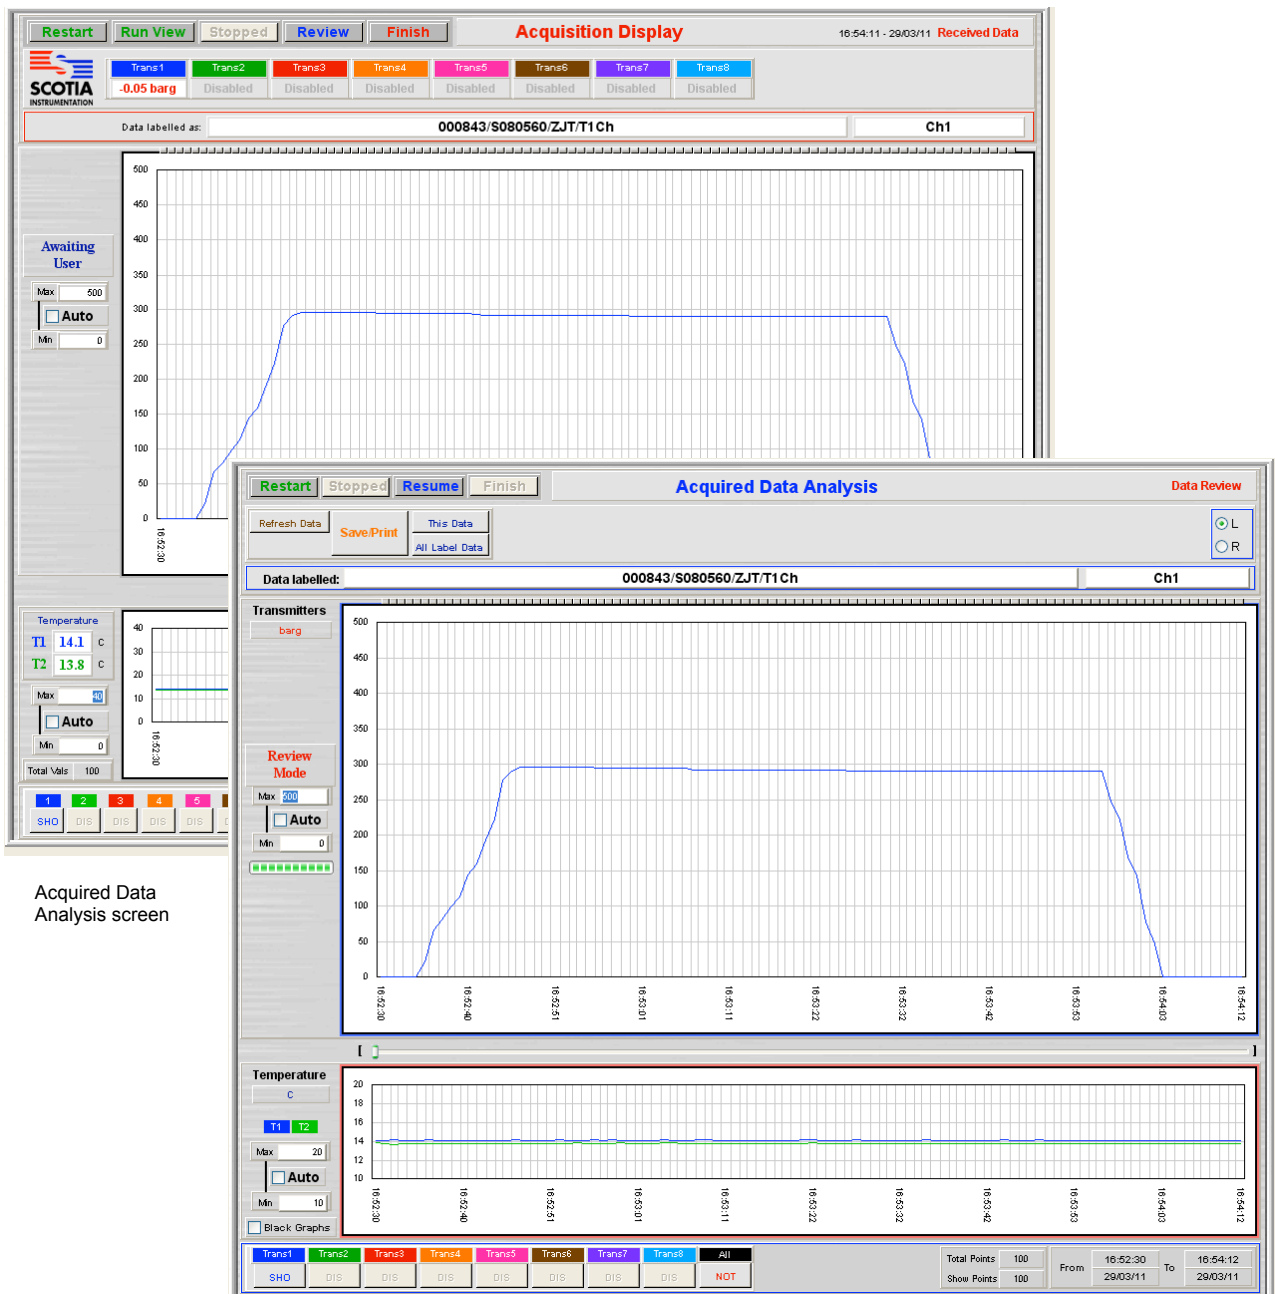

Acquired Data Analysis screen


Reduce the test period to the hold period

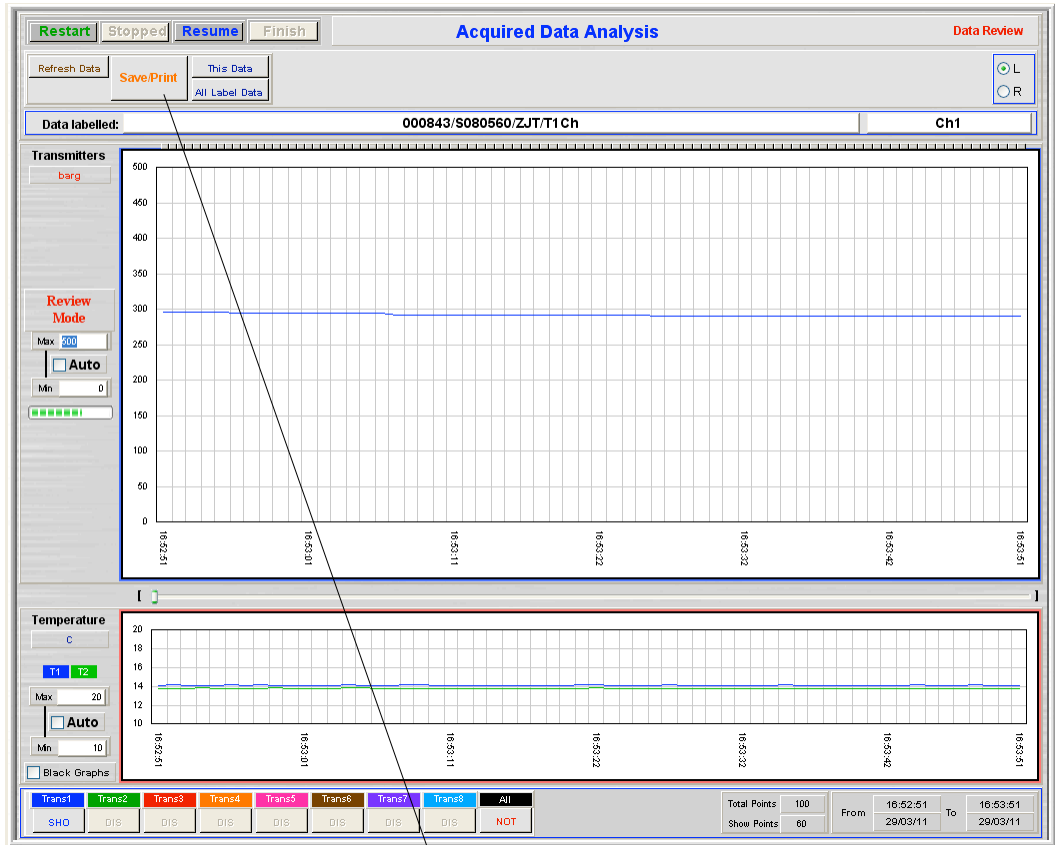

Choose Save Graph

This must be a single line graph for Certificate creation

Choose Create Cert to proceed to create a Certificate.

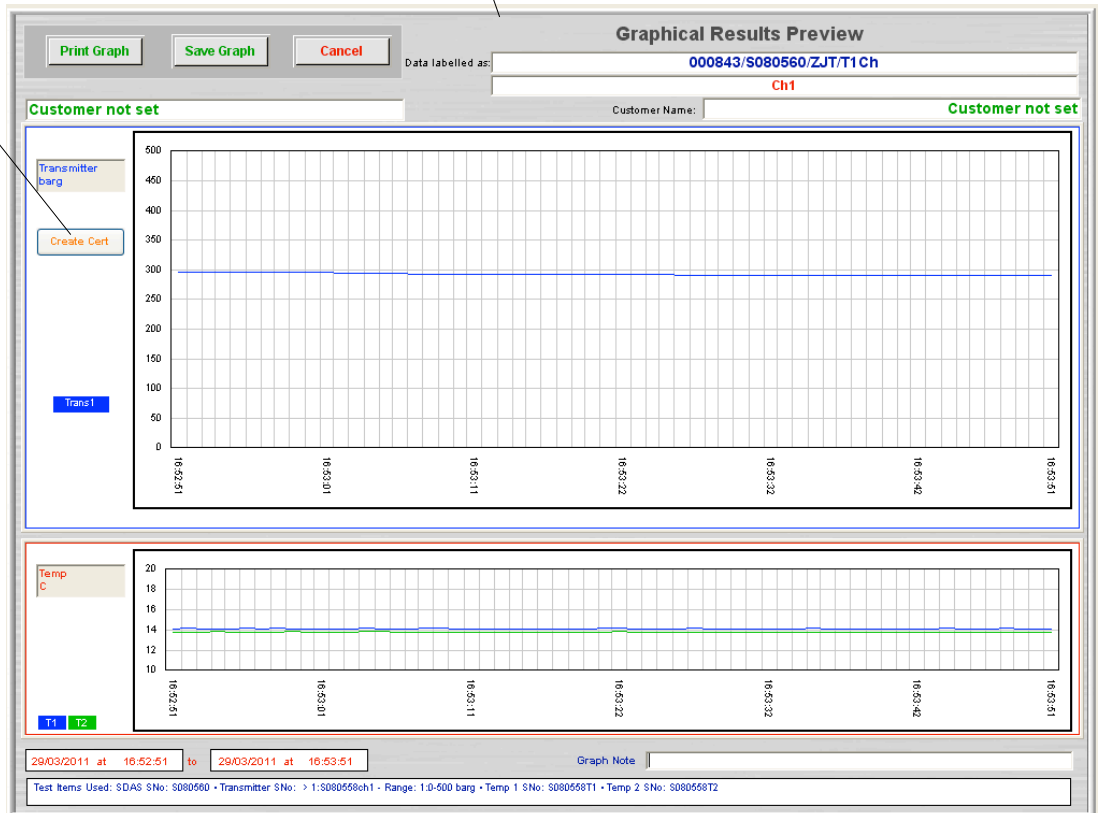

Note that if you have not created the Certificate Labels at this stage then you cannot proceed. If you have a Certificate already created for this Test then this button shows Modify Cert. You can only have one certificate for each test.

Hydrostatic Test Inspection Certificate 2

Enter or change the Certificate Details below Type 2

Scotia Instrumentation Ltd
Campus 1 - Aberdeen Science Park - Aberdeen - AB22 8GT

Client Name	Client Name
Customer	Customer name
Client Job Number	ABC123
SDAS Data Label	000843/S080560/ZJT/T1Ch : Ch1
Items Inspected	Detail of item
Drawing No(s)	A6564
Spool No(s)	S9876 S9877
Spool No(s)	

Location	South Yard
Test Type	Hydrostatic
Test Pressure	295 barg
Test Medium	Water
Test Duration	1 minute

	Time	Date	Pressure barg	Temperature
Test On	16:52:51	29/03/11	296.57	14.1
Test Off	16:53:51	29/03/11	290.93	13.8

SDAS Serial Number	S080560
Pressure Transmitter	> 1:S080558ch1
Range	1:0-500 barg
Traceable Standard	UKAS Lab 0208
Temperature Probe Serial No	S080558T1
Our Company	

Signed By	James Thom	Certificate Date	29/03/2011
-----------	------------	------------------	------------

Stop
Print & Save
Save Only

The Client, Test No, and Test On and off times and pressures are pre-filled taken from the ends of the graph defined by the user.

The test equipment detail, user and current date are also pre-filled.

Other detail needs to be filled by the user.

Data with a white background can be altered by the user.

This does not save the data entered

This brings up the normal print dialogue before printing and then saves the data entered in the Certificate file. The print is in the form shown as follows

This saves the data entered in the Certificate file

The printed certificate looks like this

Hydrostatic Test Inspection Certificate

Scotia Instrumentation Ltd
Campus 1 - Aberdeen Science Park - Aberdeen - AB22 8GT

Client Name	Client Name
Customer	Customer name
Client Job Number	ABC123
SDAS Data Label	000843/S080560/ZJT/T1Ch : Ch1
Items Inspected	Detail of item
Drawing No(s)	A6564
Spool No(s)	S9876 S9877
Spool No(s)	

This is to certify that the above items were tested as outlined below and found to be acceptable—

Location	South Yard
Test Type	Hydrostatic
Test Pressure	295 barg
Test Medium	Water
Test Duration	1 minute

	Time	Date	Pressure barg	Temperature
Test On	16:52:51	29/03/11	296.57	14.1
Test Off	16:53:51	29/03/11	290.93	13.8

Equipment Used in Test	Equipment Data
SDAS Serial Number	S080560
Pressure Transmitter	> 1:S080558ch1
Range	1:0-500 barg
Traceable Standard	UKAS Lab 0208
Temperature Probe Serial No	S080558T1
Our Company	

Signed By	James Thom	Accepted by:	Accepted by:
Our Company		Company:	Company:
Signature		Signature:	Signature:
Date	29/03/2011	Date:	Date:

SDAS Ref: 000843/S080560/ZJT/T1Ch Produced from Scotia Data Acquisition System SDASS




The logo used is set in the Utilities menu

The test certificate prints out on A4 paper



When the certificate is printed or saved the screen returns to the saved Graph screen

Review Stored Certificates

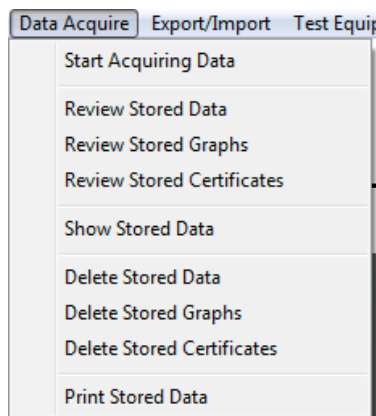

When this option is active this allows reviewing, amending and printing of a created test certificate.

Choose the search type

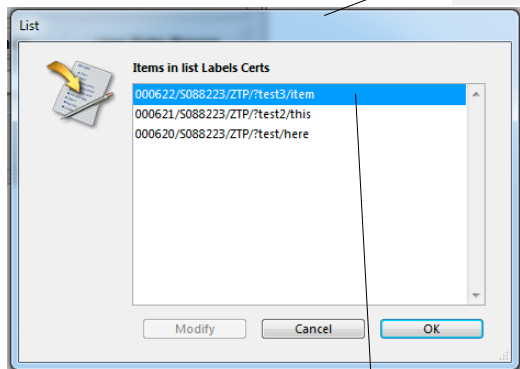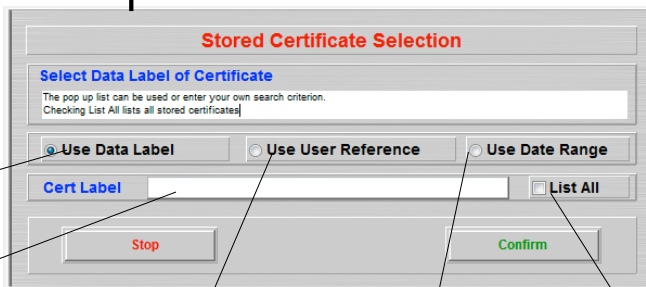

This searches for certificates with a user reference. A pop up list of saved user references is displayed

This allows a date or a range of dates to be entered in the form 25/2/16 for a date or 25/3/16-27/3/16 for a range of dates from one to the other inclusive.


Checking this box selects all the stored certificates

With these three options more than one certificate may be found. In this case a list is then shown. Double click on the item on the list to show the certificate for viewing, amending or printing

Choose from the list presented and click OK to proceed. Only one certificate can be found for one data label


Amend Certificates

Print Certificates


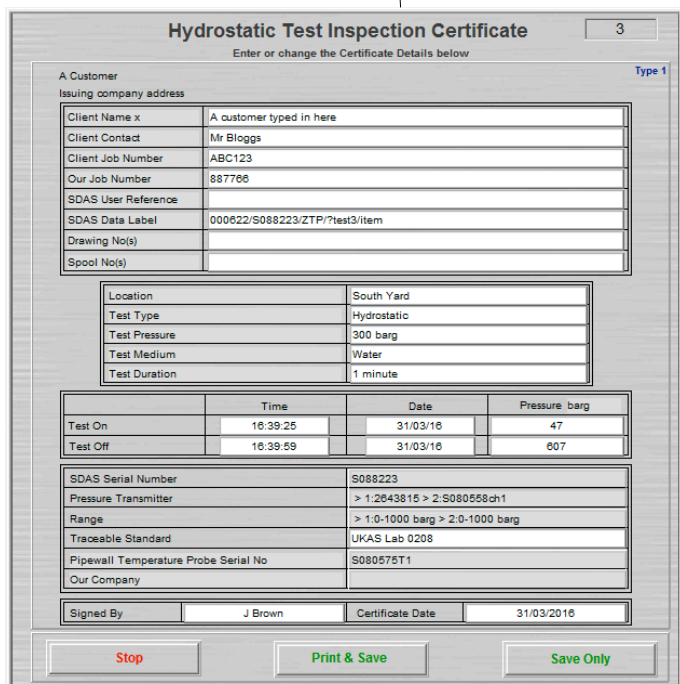


These can be amended and printed from here


Delete Stored Certificates

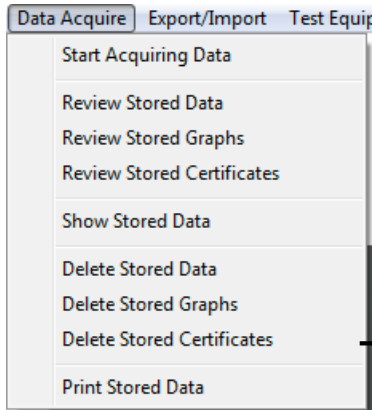

When this option is active this allows deleting of a created test certificate.

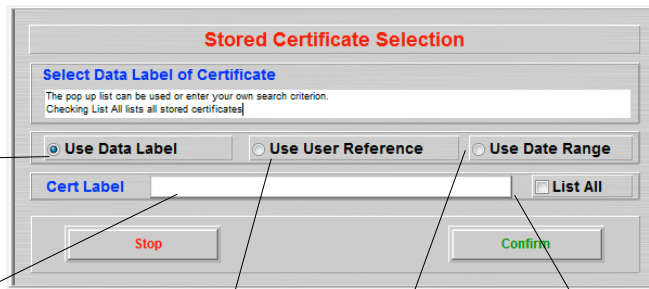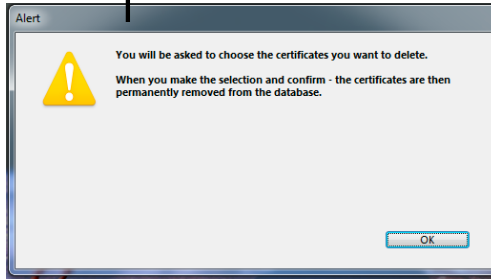

Choose the search type

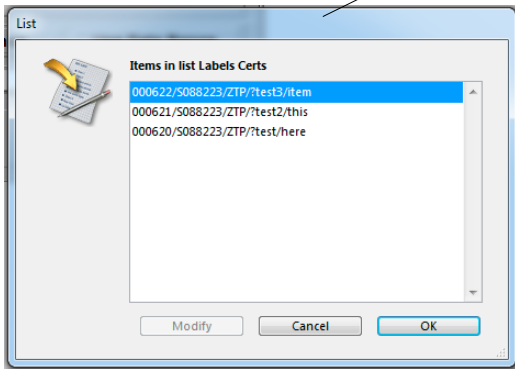


Choose from the list presented and click OK to proceed.

This searches for certificates with a user reference. A pop up list of saved user references is displayed

This allows a date or a range of dates to be entered in the form 25/2/11 for a date or 25/3/11-27/3/11 for a range of dates from one to the other inclusive.

Checking this box selects all the stored certificates

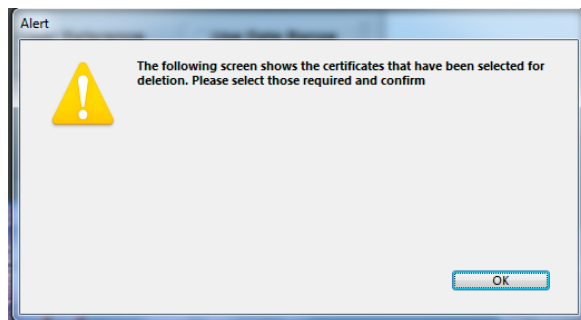

A list of the matching certificates is then shown. Double click on the item on the list to show the certificate for viewing. Any left on the list when Continue is clicked will be deleted after confirmation.

Certificate Listing

Select from the list below by clicking - shift clicking or control clicking.
Reduce the selection to those required by clicking Reduce Selection.
View/Amend/Print Certificates by Double-clicking on the one required.

Cert ID	Ident	Date	Status
3	000622/S088223/ZTP/?test3/item	31/03/2014	Imported 14/07/2018

These sort the column above them up or down

Finish **Reduce Selection** **Continue**


This stops this routine

This reduces the selection to only the certificates chosen. Highlight those required by clicking, shift clicking or control clicking

This continues this routine

You get one final chance to stop the deletion.

Confirm




OK = Delete the selected certificates
Cancel = Reconsider this action

The certificates are not deleted



No more chances after this. The certificates are gone.

Export Certificate File

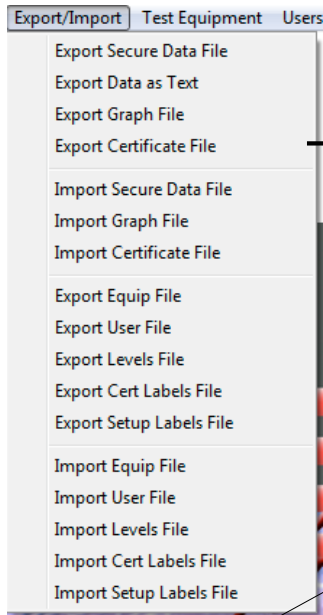

When this option is active this allows exporting of a created test certificate.

The certificate data file exported by this routine is in a form that can only be read by the Import Certificate File routine and cannot be viewed or changed by other programs. The certificate file cannot be exported as text.

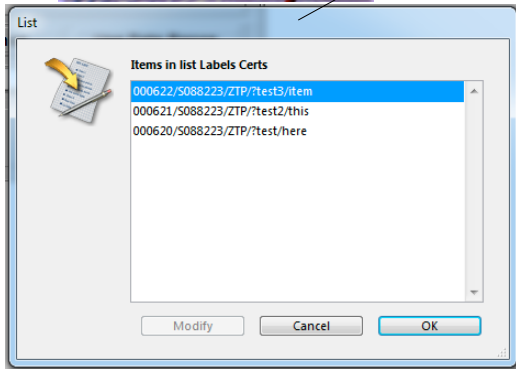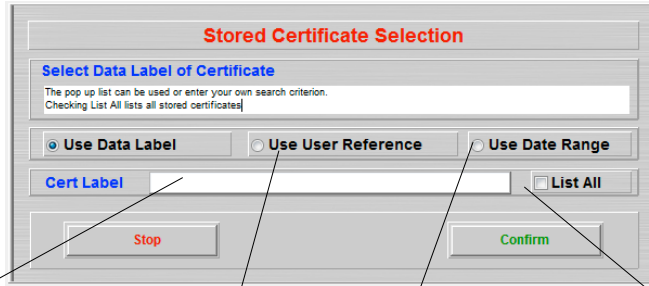


Choose from the list presented and click OK to proceed.

This searches for certificates with a user reference. A pop up list of saved user references is displayed

This allows a date or a range of dates to be entered in the form 25/2/11 for a date or 25/3/11-27/3/11 for a range of dates from one to the other inclusive.

Checking this box selects all the stored data

You are then shown a list of certificates for export

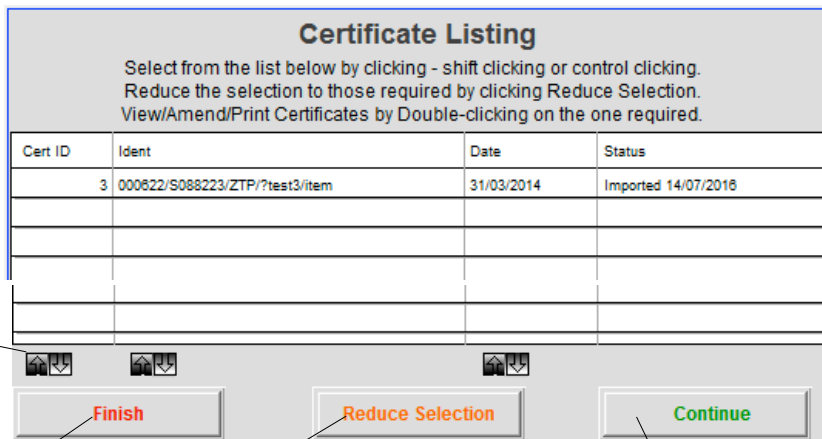

These sort the column above them up or down

This stops this routine


This reduces the selection to only the certificates chosen. Highlight those required by clicking, shift clicking or control clicking

This continues this routine

Note that all the listed certificates will be exported. You need to reduce the selection to the certificates you wish to export.


The certificate files are saved to the default saving location

Import Certificate File

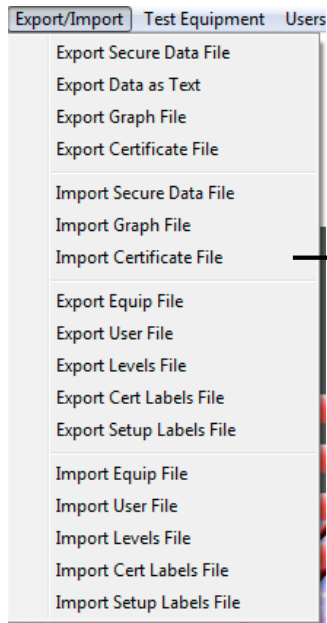


When this option is active this allows importing of an exported test certificate file. The files for import must be in the Default Load folder and start with 'C-' for this routine to load them.


The certificate data file imported by this routine is in a form that can only be read by the Import certificate File routine.

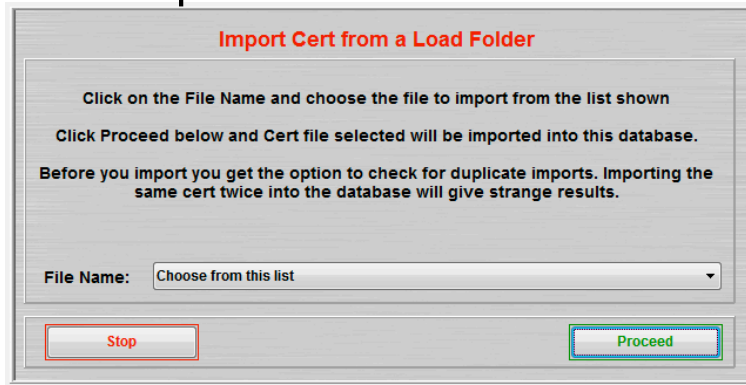

The files for import must be in the Load folder. If the file header is incorrect the import will terminate.

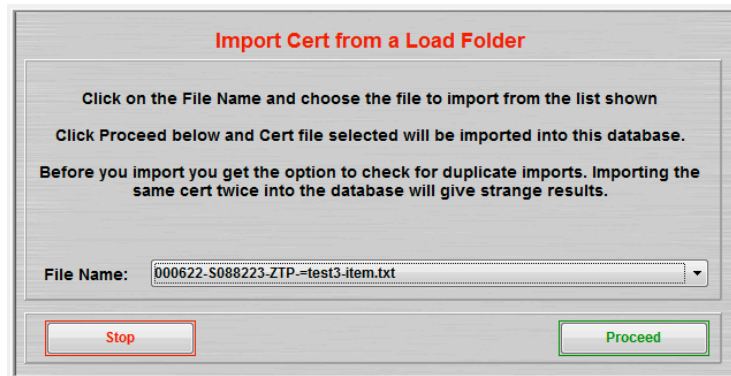


If the file is already in the database then this message appears

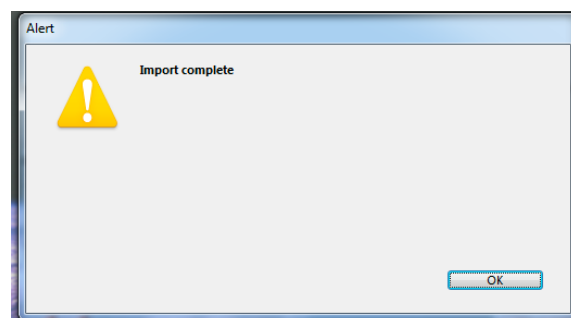


Door Alarm Option

When this option is active this allows a switch to be connected to any test bay function. Initially this was designed to alert the users to the door to the testing bay being open but it could alert the user to any action operating this switch.

When activated while logging, the user is alerted by a screen indication which covers a large section of the logging graph screen. An audible or visual alarm can also be connected to the SDAS which can be used to supplement this warning.

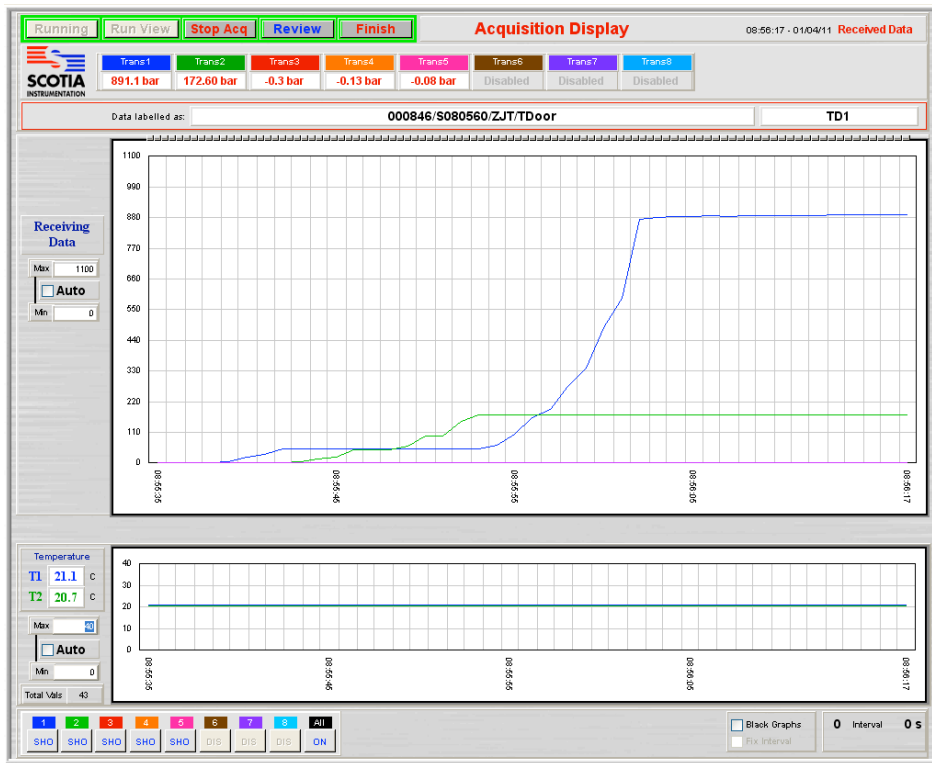

With logging in progress as above, if the switch goes 'open' then this alert appears and an audible alarm sounds

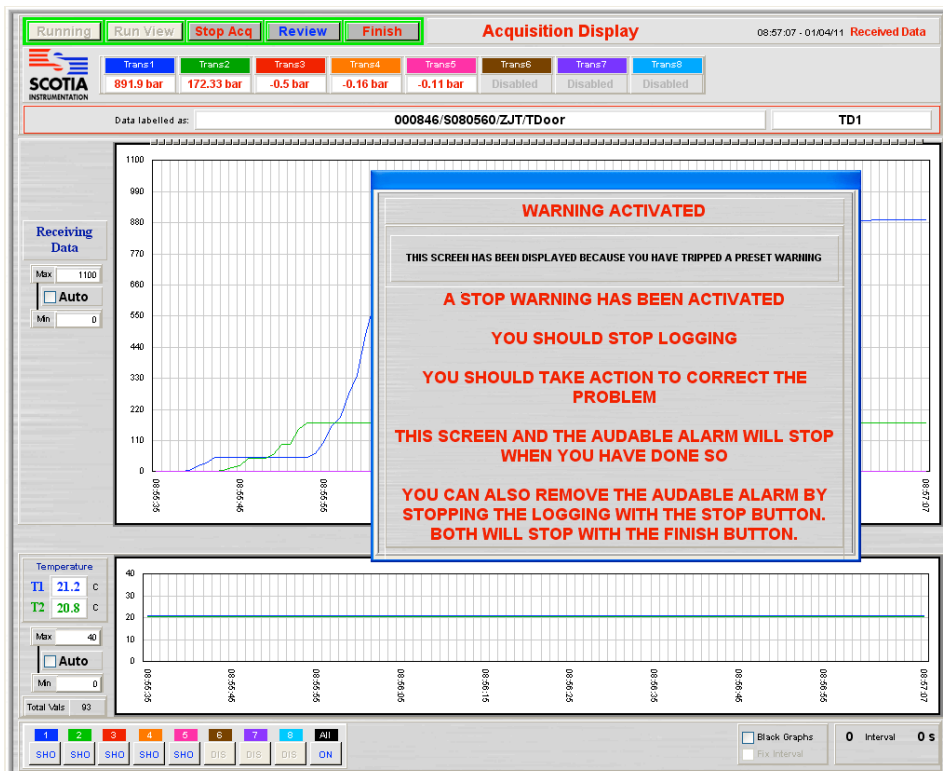

Logging continues while the alarm sounds and the screen alert shows. This alarm is recorded in the Event log. The alarm can be cancelled by closing the switch. The audible alarm will stop if the Stop Acq button is clicked. The alarm will stop and the screens will close when the Finish button is clicked.

Test Event Marking Option

This allows the user to mark a point on the logging chart and make a note to indicate why that point has been marked. The marked point shows on the logging screen as if a value has been applied to that channel and then removed. With only a few data points on the chart this shows as an inverted V but with more points the v narrows until it appears to be a single vertical line.


The marker channel is labelled as such and can be set to any value to allow the user to vary the height of the marker as it marks to 20% of its range. The range and units of the marker channel should match the channels to be marked. Test Event Marking requires a hardware addition of a TME plug and this uses one of the SDAS channels. The TME plug must be added to the SDAS Test Equipment list with the serial number 'Markplug'.

The marked points can be viewed and read in the Review mode. Moving the slider control to a marker point pops up the marker message for that point.

When printing a chart the notes from the markers print on an A4 page following the printing of the chart page.

Marks and their notes are saved with the test data for recovery later or for export to SDAS Review software.


Click Create Mark to start the process. The Marker channel gets a value of 20% of its range and the data screen appears and remains floating over the Acquisition Display screen until the user clicks the 'Save + Close' button. The floating screen can be moved to another location by clicking and dragging the window banner.

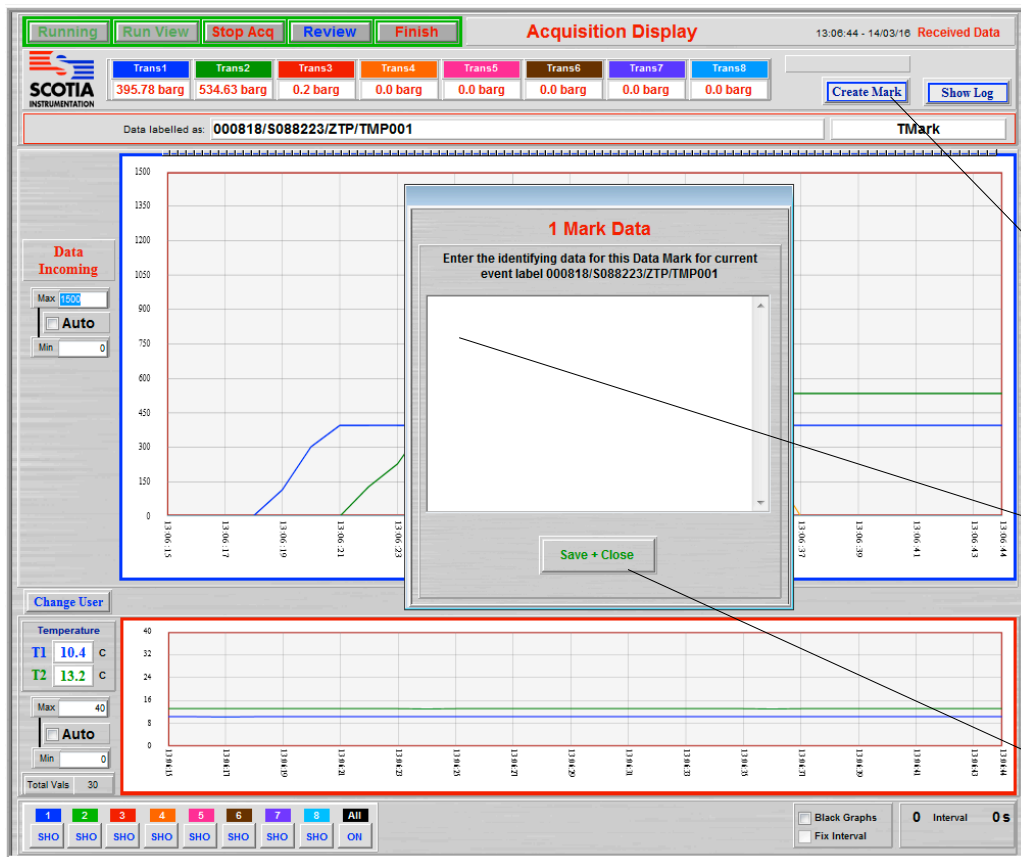

Click Create Mark to create the mark and bring up the entry screen


Enter the mark description message here

Click Save + Close to confirm your entry and close the window

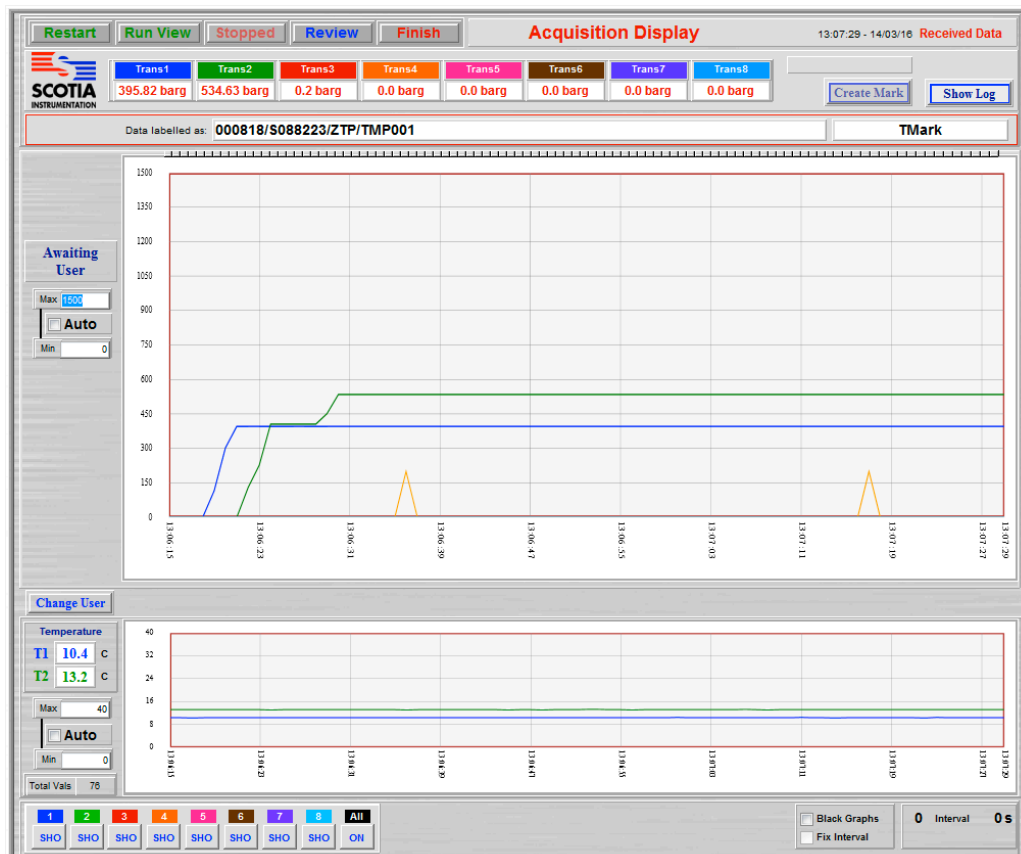


Two data marks have been added as an example

Click Review to see this screen then insert the Location Marker or move the Slider until it is at the Mark. The Mark data pops up. When a lot of data points are showing on the Review graph, the exact point for the Mark may be hard to click on. Click near it and move the Slider one point at a time by using the [] keys to get the Mark point. The Mark Data message is removed by the system after a few seconds.

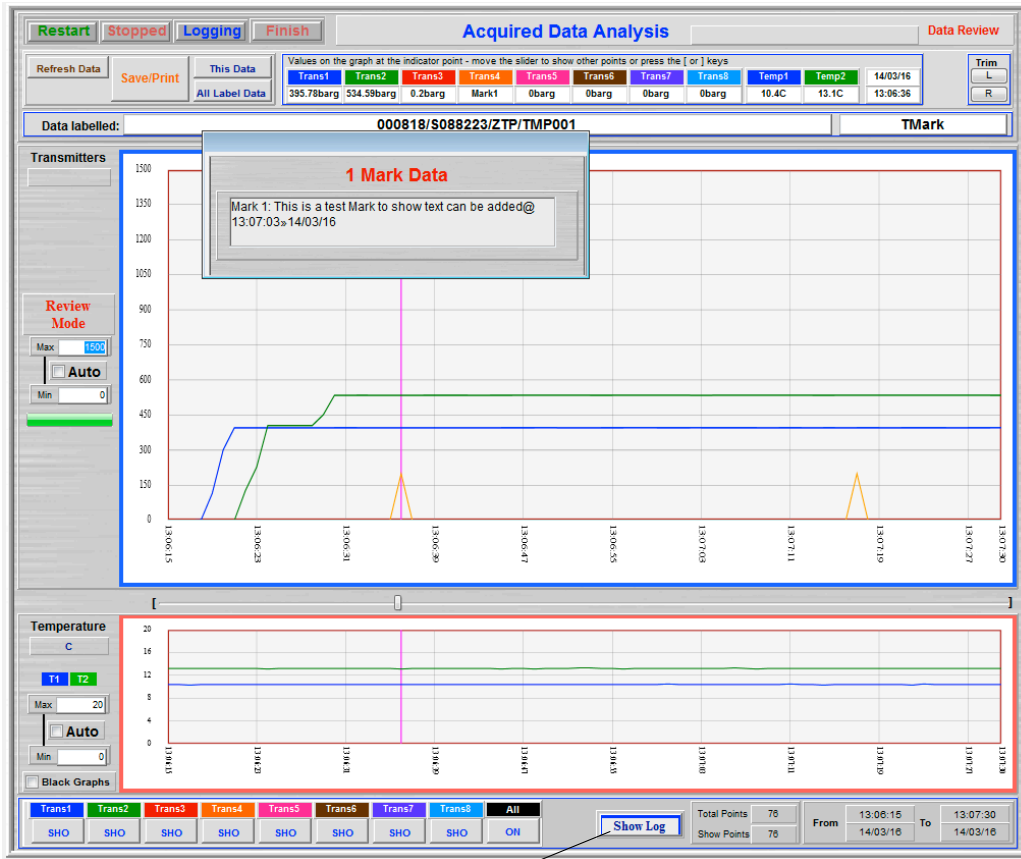

All the Mark data along with other event logs shows when the Show Log is clicked

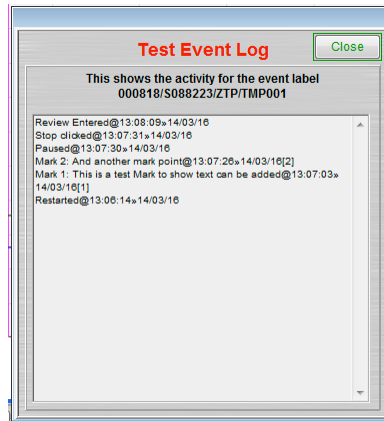

When the test chart is printed any Mark data is printed after the main print page with all the Mark data. Note that this will print all the Mark data entries not just those showing on a section of the data should only a section of the data be printed.

Enhanced Data Entry Option

The new data pallet offers enhanced user data labeling for tests on the SDAS units

This not only allows users to input more data to label the test output results form but they can search by those items of data in addition to the current SDAS search routines.

Data can also be uplifted to the SDAS units directly from a text file stored locally to the SDAS or a network location. This data file is a standard tab delineated text file which can produced from most computer systems. This allows the labeling data to be prepared externally to the SDAS and simply imported by the user reducing the user input burden and eliminating any typing errors. This file must be prefixed with 'SUD-' and be placed in the default Load folder in order for the loading routine to find it. A list of those found will be shown for choosing.

The SDAS still retains its unique test IDs which are saved in addition to any other data.

There are nine data fields provided which can be labelled by the user in any way. These labels are saved with the data allowing them to be recalled with their associated data. Any subsequent changes to the data labels are saved for future entries without affected previous ones. Data labels can be exported to be read by other SDAS units.

The additional data fields together with their labels are printed on the test output results form.

This data pallet function can be toggled on/off. When off the SDAS returns to the original version 6 appearance, functions and printouts.

The labels for the data pallet must be set up in Settings menu or added via Import before you start data gathering or the system will stop until you do.

Currently this option is linked with the Hold Period Tracking option.

The additional data for a test can be entered in three ways in the following screen. The data can be keyed in by the user. Any entries left blank are not included in the test output results form. The data can be copied from a previous test by selecting the Data Label from the pop up list of previous tests. The data can be loaded from a prepared tab delineated text file by clicking Load File.

Test Set Up Data
Enter or import the test data below

The Data Label is used as a part of the test label

Data Label:

Click on the Document Name below and select the preset data that you want to import

Document Name: Choose from this list

Test Data Entry:

Use of space / - + = are not allowed here as they are reserved for system use

<input checked="" type="checkbox"/>	Sales ONo	
<input checked="" type="checkbox"/>	Works ONo	
<input checked="" type="checkbox"/>	Part No	
<input type="checkbox"/>	Serial No	
<input type="checkbox"/>	Proc No	
<input type="checkbox"/>	Proc Section	
<input type="checkbox"/>	Cust Name	
<input type="checkbox"/>	Operator	
<input type="checkbox"/>	Inspector	

Manual entries above must be confirmed by clicking Fill Label

Buttons: Stop, Proceed

Annotations:

- The labeling of the data can be set and altered by the user. The labels are saved with the test data
- Data items checked here will have this data entered in the main Data Label. The choice of items to be included is saved for the next entry.
- Data can be entered manually in each field. Any fields left blank are ignored for the final test output.
- A stored text file can be loaded by clicking on the popup list and choosing the one required
- If data is entered manually the user must click Fill Label to proceed. Any spaces will be replaced by underline when entered in the Data Label

Test Set Up Data
Enter or import the test data below

The Data Label is used as a part of the test label

Data Label: Test1/file_entry_2/file_entry_3

Click on the Document Name below and select the preset data that you want to import

Document Name: test1.txt

Test Data Entry:

Use of space / - + = are not allowed here as they are reserved for system use

<input checked="" type="checkbox"/>	Sales ONo	Test1
<input checked="" type="checkbox"/>	Works ONo	file_entry_2
<input checked="" type="checkbox"/>	Part No	file_entry_3
<input type="checkbox"/>	Serial No	file entry 4
<input type="checkbox"/>	Proc No	file entry 5
<input type="checkbox"/>	Proc Section	file entry 6
<input type="checkbox"/>	Cust Name	
<input type="checkbox"/>	Operator	
<input type="checkbox"/>	Inspector	

Manual entries above must be confirmed by clicking Fill Label

Buttons: Stop, Proceed

Annotations:

- Click Stop to abort this process and return to the main screen.
- Click Proceed to continue
- Sample data entered - note that only the lines ticked have been used for the Data Label

Hold Period Tracking

Observing a pressure drop over time looking for an allowed drop in a given time - eg an allowed 5 barg drop over 30 minutes. The data pallet when activated in the Drop mode is looking for allowed criteria. It will monitor the pressure over time giving on screen progress indication. This will show the current drop rate and indicate whether this is on target or not. When the drop period has passed with an allowable drop value the test will show a pass. If not then the time window will move noting the value at the start and finish of the moving time window. When a pass is calculated then this will be indicated.

The test monitoring can be set to either stop automatically at a pass or indicate to the user that a pass has been noted and ask the user to indicate the pass should be accepted. Once accepted the start/finish values and time/date of the event are noted together with the name of the user accepting the test. These are printed on the test output results form.

If Data Pallet has been chosen to be active the following screen appears in the loading sequence. The test criteria for the Data Pallet can be entered in two ways in the following screen. The data can be keyed in by the user. The data can be reloaded from a previous test or from a prepared tab delineated text file by choosing from the Document Name popup list

Manual entry is started by clicking here and choosing the test type.

Select the channel number to be used for this test

Enter the hold period in minutes

Enter the allowed drop in the units of channel used

Enter the minimum value for the test in the units of channel used. If this check is not required then set a value lower than any expected.

A stored text file can be loaded by clicking and selecting from the popup list

Auto End will stop this part of the Hold Period tracking as soon as the criteria are met and note the result points. Unchecked will mean the user will need to confirm when the test is complete.

Any test not active will be ignored by the system. If no steps are active then the Data Pallet will be disabled in the gathering screen.


Enter a file name and click Save Data to save the Test Steps as currently displayed. These can then be reloaded for future tests.

Click Stop to abort this process and return to the main screen.

Click Proceed to continue

If Data Pallet has active test steps then the Show Pallet button appears. When this button is clicked the Data Pallet appears and runs the first active test. The pallet appears to float over the normal screen and can be moved to any location on the screen. The system will remember this location and will show the pallet in this location the next time it is opened.

It is expected that the pallet will be activated when the user is ready to evaluate the received readings. Measuring a Hold period is not expecting to find transmitter values increasing. Evaluation will be interrupted if rising values are detected.

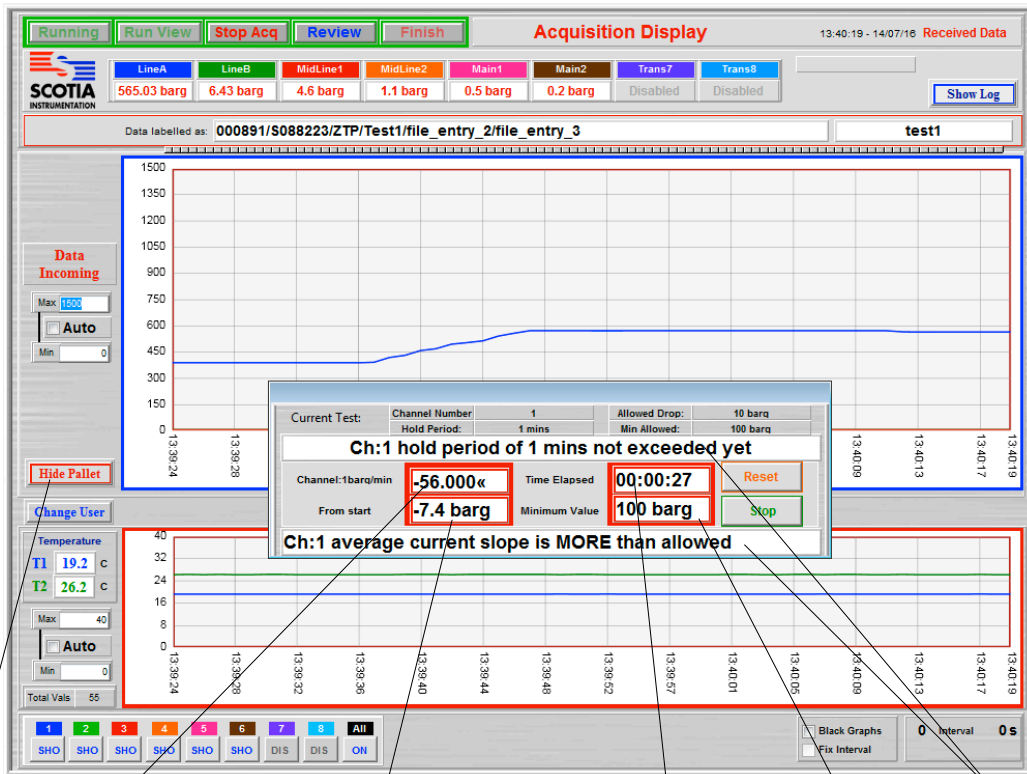

The Show Pallet button changed to Hide Pallet when the Data Pallet appears

The slope of the indicated channel is calculated from an average of 10 readings. The slope value appears after this countdown.

The change from the start of the evaluation is shown until the hold period is reached and then the change from the start of the rolling hold period is shown

The time from the start of this evaluation is shown


The minimum value allowed for the test is shown here.

Information on the test is shown here


Clicking Reset at any time will restart the evaluation period again

The test criteria are shown along the top of the floating screen

When the evaluation starts the data must gather for 10 seconds to achieve an average value.

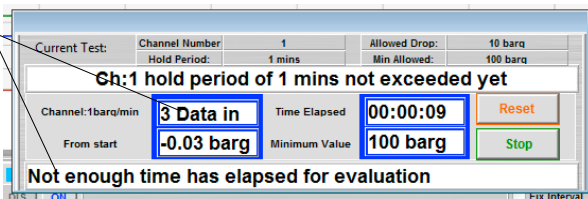

The progress of the evaluation is shown

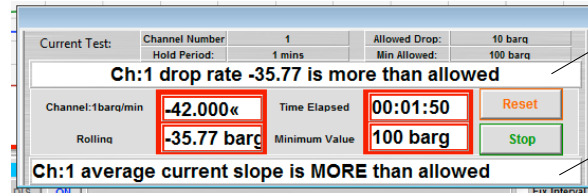


The current drop rate is shown

The screen flashes red to indicate a fail situation currently


The slope of the currently received data is evaluated as a forward projection. At this point the projection is that the test will fail

The screen now flashes green to indicate a pass is expected if the rate of fall does not change

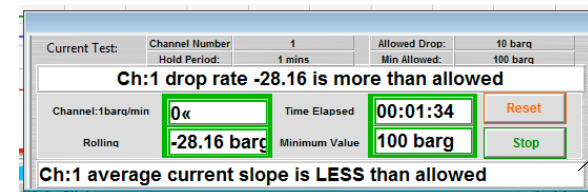


The current drop rate is shown

The slope of the currently received data is evaluated as a forward projection. At this point the projection is that the test will pass but the drop rate in the time set has been exceeded

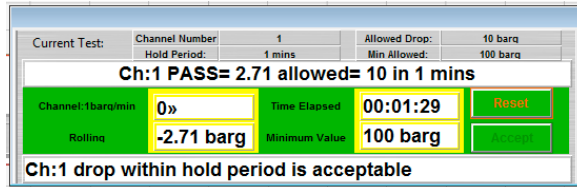


The screen now flashes green to indicate a pass situation but the evaluation continues until the operator clicks Accept

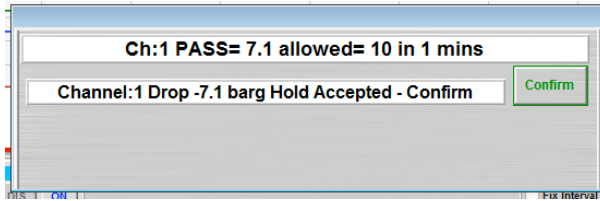

If Auto End had been selected at the start then this screen would have appeared whenever the routine detected the pass criterion

The test even log shows the start and finish values with the drop test criteria

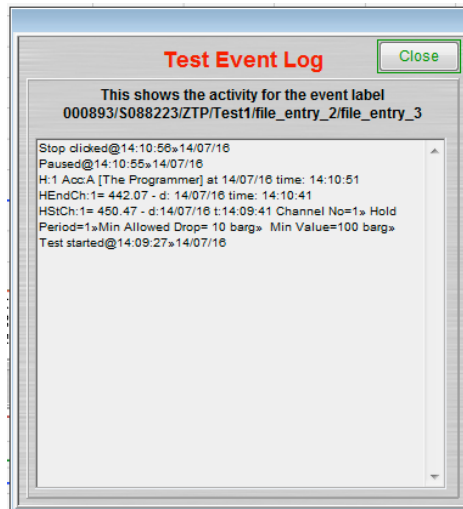

Peak Value Tracking

Observing the maximum value. The system can detect the maximum value in a channel over a period. This can be done automatically or manually. In automatic the system will stop monitoring and note the value as soon as it detects a value lower than the previous one. In manual mode the system keeps looking for a maximum until the user accepts. It then records the maximum value it has noted from the start of the observing period. The user can reset the tracking period at any time.

If Data Pallet has been chosen to be active the following screen appears in the loading sequence. The test criteria for the Data Pallet can be entered in two ways in the following screen. The data can be keyed in by the user. The data can be copied from a previous test or from a prepared tab delineated text file by selecting Load Data.

Test Step Set Up

Complete the test criteria and sequence below to proceed

Allowed drop values set must be in same units as the channel values in Channel No set
 Allowed Drop is the amount of decrease in the channel value over the set Hold Period
 Allowed drop values are given as a positive value
 Hold Period is given in minutes
 Minimum value is the lowest value allowed for the test. Value must be in the same units as channel
 When Auto End is checked the step will end without operator action when the test criteria are met

Choose by clicking on the test type below to start the process

Test Step	Test type	Ch No	Hold Period	Allowed Drop	Min Value	Auto End	Active
1	Peak	1	0	0	0	<input type="checkbox"/>	<input checked="" type="checkbox"/>
2		0	0	0	0	<input type="checkbox"/>	<input type="checkbox"/>
3		0	0	0	0	<input type="checkbox"/>	<input type="checkbox"/>
4		0	0	0	0	<input type="checkbox"/>	<input type="checkbox"/>
5		0	0	0	0	<input type="checkbox"/>	<input type="checkbox"/>
6		0	0	0	0	<input type="checkbox"/>	<input type="checkbox"/>

Leaving no Active Steps will disable the Data Pallet function on the data gathering screen

Select from the Document Name below to load test setup stored data from the TestData folder

Document Name: Peak1

Test steps entered above can be saved in the TestData folder for reload by entering a name below and clicking Save Data

File Name: Save data

Stop Proceed

Manual entry is started by clicking here and choosing the test type.

Select the channel number to be used for this test

Any test not active will be ignored by the system. If no steps are active then the Data Pallet will be disabled in the gathering screen.

A stored text file can be loaded by clicking and selecting from the popup list

Test Step Set Up

Complete the test criteria and sequence below to proceed

Allowed drop values set must be in same units as the channel values in Channel No set
 Allowed Drop is the amount of decrease in the channel value over the set Hold Period
 Allowed drop values are given as a positive value
 Hold Period is given in minutes
 Minimum value is the lowest value allowed for the test. Value must be in the same units as channel
 When Auto End is checked the step will end without operator action when the test criteria are met

Choose by clicking on the test type below to start the process

Test Step	Test type	Ch No	Hold Period	Allowed Drop	Min Value	Auto End	Active
1	Peak	1	0	0	0	<input type="checkbox"/>	<input checked="" type="checkbox"/>
2		0	0	0	0	<input type="checkbox"/>	<input type="checkbox"/>
3		0	0	0	0	<input type="checkbox"/>	<input type="checkbox"/>
4		0	0	0	0	<input type="checkbox"/>	<input type="checkbox"/>
5		0	0	0	0	<input type="checkbox"/>	<input type="checkbox"/>
6		0	0	0	0	<input type="checkbox"/>	<input type="checkbox"/>

Leaving no Active Steps will disable the Data Pallet function on the data gathering screen

Select from the Document Name below to load test setup stored data from the TestData folder

Document Name: Peak1

Test steps entered above can be saved in the TestData folder for reload by entering a name below and clicking Save Data

File Name: Save data

Stop Proceed

These are not active when the test type is Peak

Auto End will stop this part of the data pallet as soon as the criteria are met. Unchecked will mean the user will need to confirm when the test is complete.


Enter a file name and click Save Data to save the Test Steps as currently displayed. These can then be reloaded for future tests.

Click Stop to abort this process and return to the main screen.


Click Proceed to continue

If Data Pallet has active test steps then the Show Pallet button appears. When this button is clicked the Data Pallet appears and runs the first active test. The pallet appears to float over the normal screen and can be moved to any location on the screen. The system will remember this location and will show the pallet in this location the next time it is opened.

The start or reset settles for 3 seconds and counts down showing the channel being tracked and the current value

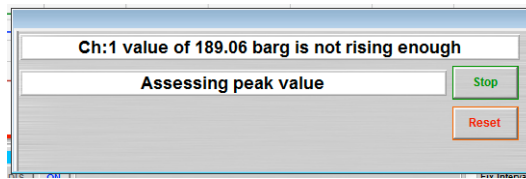

When the peak assessment is activated and the monitored value is not rising enough this screen shows

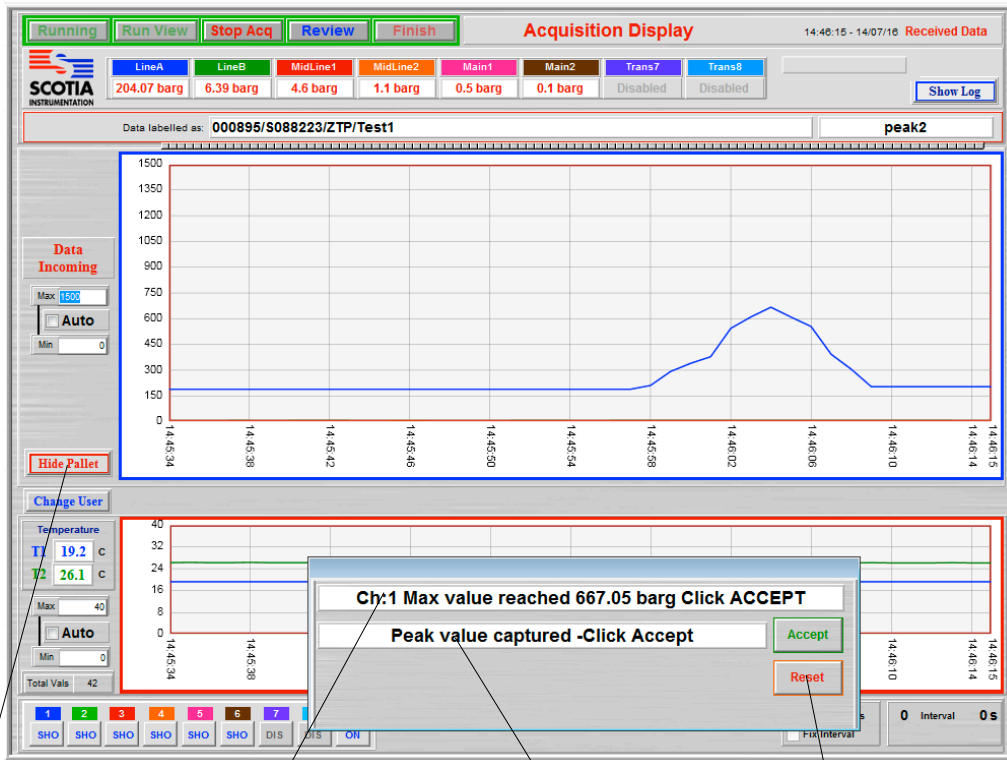


The Show Pallet button changed to Hide Pallet when the Data Pallet appears

The start or reset settles for 3 seconds and counts down showing the channel being tracked and the current value

The current status is shown here

Reset restarts the peak tracking and will start noting the peak value received from that point

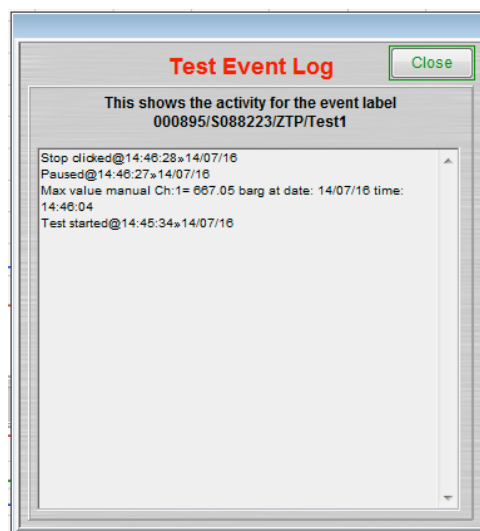

The test event log shows the maximum value

If the Peak Tracking is not set to automatically end then the routine continues to monitor the peak value and updates it on screen. When Accept is clicked it records this value. Reset can be clicked at any time and the system will capture the peak value from that point.

Test Combining

Up to six routines combining these two can be loaded and run. These routines can be entered and saved for future tests. These routines can also be uplifted to the SDAS units directly from a text file stored locally to the SDAS or a network location.

Tests can be combined to run a sequence of tests. One test completing leads on to the next test in the sequence.

Test Step Set Up

Complete the test criteria and sequence below to proceed

Allowed drop values set must be in same units as the channel values in Channel No set
 Allowed Drop is the amount of decrease in the channel value over the set Hold Period
 Allowed drop values are given as a positive value
 Hold Period is given in minutes
 Minimum value is the lowest value allowed for the test. Value must be in the same units as channel
 When Auto End is checked the step will end without operator action when the test criteria are met

Choose by clicking on the test type below to start the process

Test Step	Test type	Ch No	Hold Period	Allowed Drop	Min Value	Auto End	Active
1	Hold	1	1	5	100	<input type="checkbox"/>	<input checked="" type="checkbox"/>
2	Peak	1	0	0	0	<input type="checkbox"/>	<input checked="" type="checkbox"/>
3	Hold	1	5	10	200	<input type="checkbox"/>	<input checked="" type="checkbox"/>
4		0	0	0	0	<input type="checkbox"/>	<input type="checkbox"/>
5		0	0	0	0	<input type="checkbox"/>	<input type="checkbox"/>
6		0	0	0	0	<input type="checkbox"/>	<input type="checkbox"/>

Leaving no Active Steps will disable the Data Pallet function on the data gathering screen

Select from the Document Name below to load test setup stored data from the TestData folder

Document Name:

Test steps entered above can be saved in the TestData folder for reload by entering a name below and clicking Save Data

File Name:

These tests will be done in this sequence

Any of the tests can be disabled by unchecking the Active box

Recalibration Due Option

This option checks the recalibration date of transmitters and temperature probes connected to the SDAS.

This can be checked by either the Test Equipment menu - Get Connected Transmitters or when the test is started.

Current Attached Equipment

These are the current Transmitters that are connected

Channel Transmitters

	Transmitter	Serial	Chip ID	Range		Cal Date	ReCal Date	Status	
Channel 1	Test CH1	S080558ch1	14786E11	0	700	barg	01/05/16	01/08/16	Passed
Channel 2	Test CH2	S080558ch2	1479B214	0	750	barg	01/02/16	01/08/16	Passed
Channel 3	Test CH3	S080558ch3	147A69C0	0	1000	barg	01/04/16	01/08/16	Passed
Channel 4	Test CH4	S080558ch4	1479AF4F	0	1000	barg	01/05/16	01/08/16	Passed
Channel 5	Test CH5	S080558ch5	147941D	0	1250	barg	01/05/16	01/01/17	Passed
Channel 6	Test CH6	S080558ch6	147834E4	0	1500	barg	01/05/16	01/06/16	Failed
Channel 7	Disabled	Disabled	Disabled	0	0	.	00/00/00	00/00/00	Disabled
Channel 8	Disabled	Disabled	Disabled	0	0	.	00/00/00	00/00/00	Disabled

Temperature Probes

Temp 1	Temp Probe	S080575T1	147A6DE2	0	100	seg C	00/00/00	01/01/17	Passed
Temp 2	Ambient Temp	S080575T2	147A5FDD	0	100	seg C	00/00/00	01/06/17	Passed

Any item with a calibration date before the current date shows Failed status

This test is run during the Start Acquiring Data routine and stops the process. The operator cannot proceed until the Recalibration date is set to a date after today or the recalibration check is toggled to off. Only QA Access users can access this menu item.

Transmitter Calibration Status

One or more of your transmitters or temperature probes are due a recalibration.

You are not allowed to proceed until the Recalibration date is after today.

You must either swap the transmitter or temperature probe for one in calibration or disable the calibration date check before you can proceed.

Transmitter	Serial Number	ReCalibration	Status
Test CH1	S080558ch1	01/08/16	Passed
Test CH2	S080558ch2	01/08/16	Passed
Test CH3	S080558ch3	01/08/16	Passed
Test CH4	S080558ch4	01/08/16	Passed
Test CH5	S080558ch5	01/01/17	Passed
Test CH6	S080558ch6	01/06/16	Failed
Disabled	Disabled	00/00/00	Disabled
Disabled	Disabled	00/00/00	Disabled
Temp Probe 1	S080575T1	01/01/17	Passed
Temp Probe 2	S080575T2	01/06/17	Passed


Stop

The user can only choose to Stop here


Export Test Data at Finish

This option exports the test data in secure data form at the end of acquiring when the Finish button is clicked. The option can be toggled on or off in the Utilities menu.

The Secure data is saved to the Default Save Location set in the Settings menu. If the path to this location cannot be seen when starting data acquiring then the following screens appear.

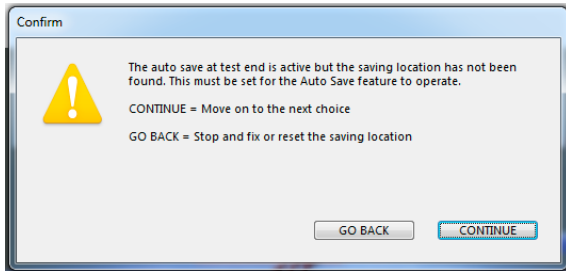


The user gets the choice to continue to the next choice or stop now and get the saving path problem fixed.

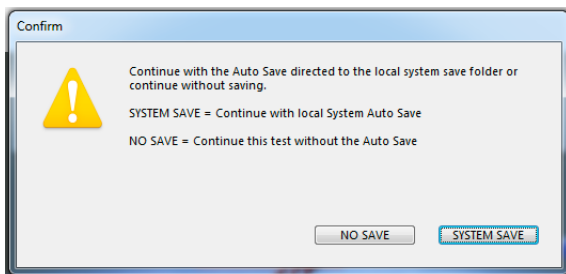


The choice is now to save to internal system save folder or proceed with export test data at finish temporarily off.

If the path the internal system save folder also cannot be found then another screen appears to say that and your only choice is to proceed without exporting data at test end. The test data is always saved within the SDAS database of course.

When you click the Finish button at the end of a test period the secure data file is exported. You are shown the following screen to confirm the export action.

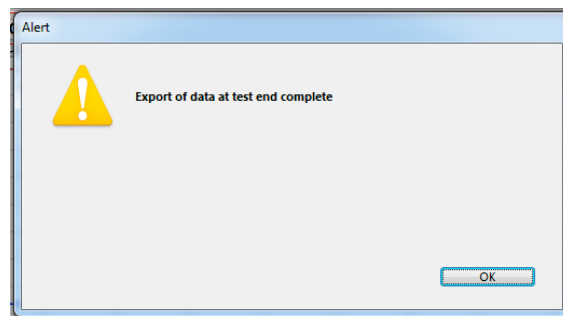

If between starting the test and the end the path to the saving location is lost then the following screen appears.

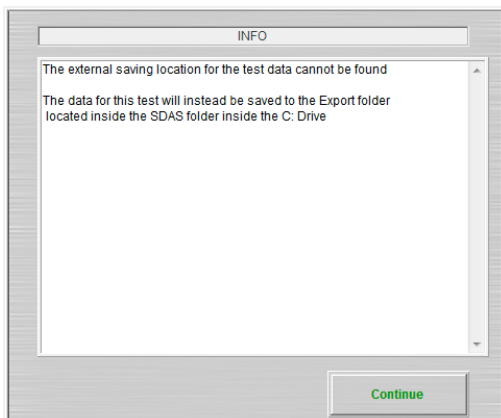

The confirmation screen then appears.

The secure data is now saved in the system save location. It can be copied out from there to another location.


The test data is still held in the SDAS database

File Browser

The File browser allows for the copying, moving and deletion of files from the local folders. It can be accessed from the File Browser selection in the Utilities menu.

By default users can only copy files. Allow delete files must be checked in the level for the user to allow them to move or delete.


This feature requires the System Save, User Save, User Load and User Test folder locations to be set in the Settings Menu.

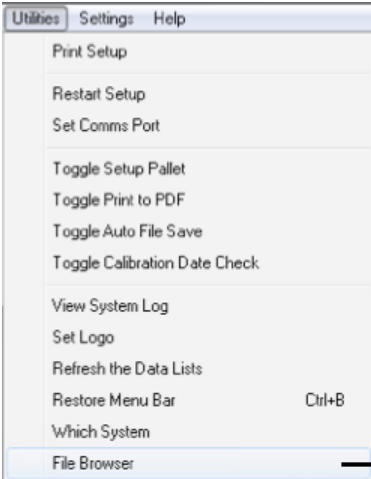


This launches a File browser which allows copying moving and deleting files exported to the System Save, Save, Load and Test folders.

If the User Save, User Load or User Test folder are set to a location not on the SDAS local hard drive deletion and moving from those folders will be disabled.


The buttons will be disabled if you cannot perform a operation either due to user level or the locations picked.

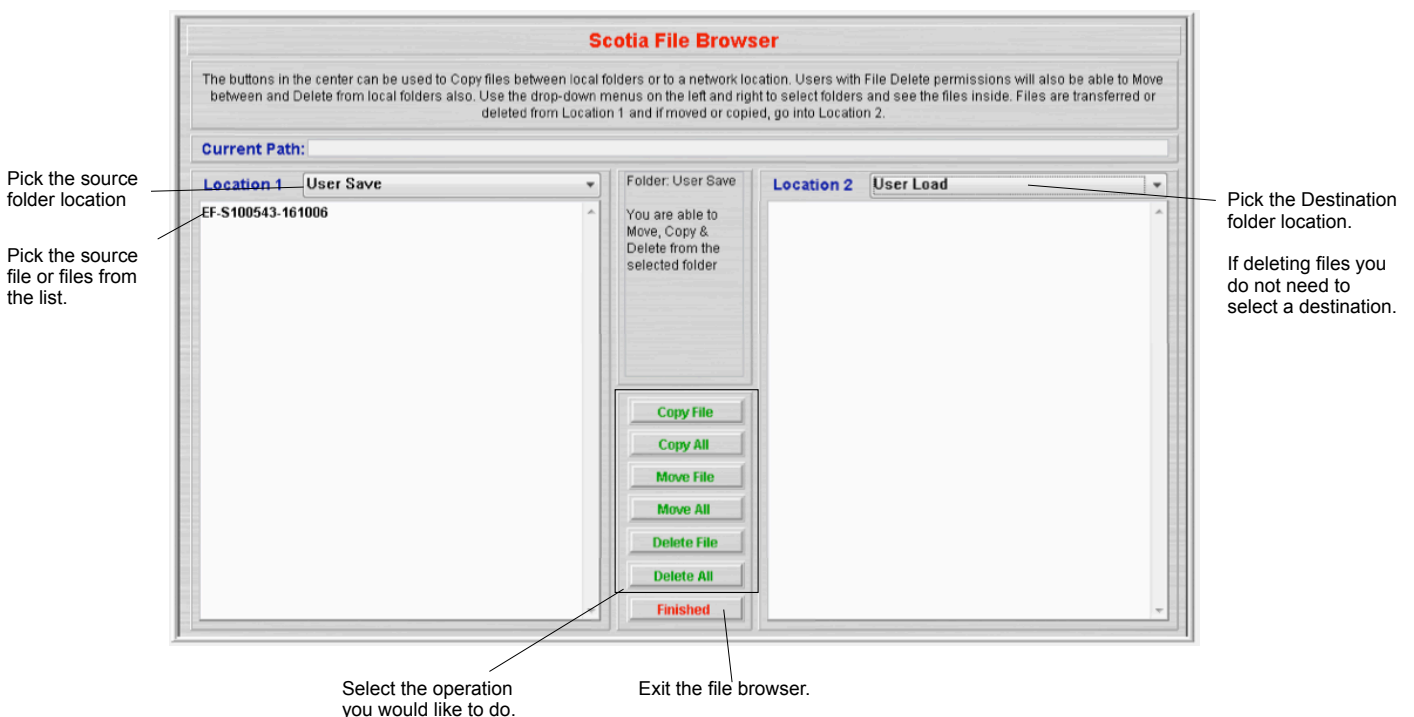

If any of the are network locations and the network location is unavailable the pick list for the locations will not show them. In the case below the Save, Load and Test folder are on a network drive that has disconnected so only the local System Save folder is available in the list.

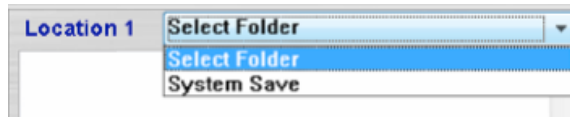

If any of the file locations have not been set properly you may see the following error message. Go to the Settings menu and set the default saving folders and default system saving location to rectify this.

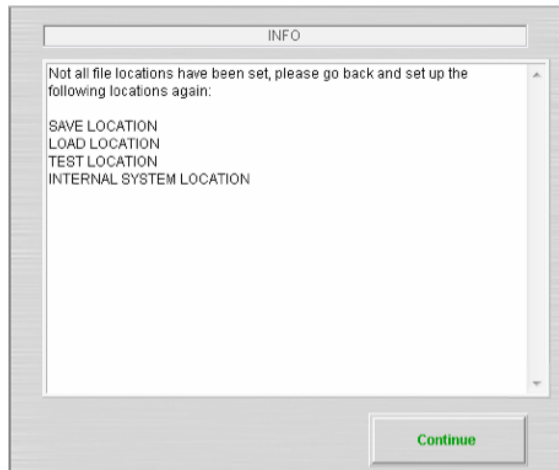

SDAS5 Hardware

SDAS5 Unit front



SDAS5 Unit back



Note that all connections below should be made prior to switching the SDAS unit on. The SDAS PC is configured to allow the user a minimum of access. Note that attaching items to ports may cause the PC to attempt to load drivers which it then cannot access. This may cause failure of the internal PC. You should have the SDAS set up to operate with any devices you intend to use by the technical staff at Scotia.



Mains Switch

Momentary green push button switch turns mains power on. Device is powered down by selecting from the screen to ensure correct power off.



Mains Power

Mains power is supplied to a IEC male socket via the mains lead supplied. Voltage in range 90 to 264 VAC 47-63 Hz. Current in range 1.1 to 2.1A depending on voltage.











Monitor Power

Monitor power is available from this IEC female socket



External Monitor

Connect the 15 way D connector from monitor to this port

Front		USB	USB 2.0/1.1. These ports can be used to attach keyboards, mouse, memory devices or printers. Note that these may have to have drivers installed prior to you plugging them in. The standard SDAS keyboard has a mousepad built in.
Rear			
		Network	Connect via RJ45 plug to network. Provides LAN connection as NIC 10/100. Note that connection to a network may require some IT input as the standard setup is via DHCP.
		TX Fuse	A 500 mA fuse protects the transmitter supply
		Alarm	With the Alarm option enabled this LED illuminates when the alarm is triggered
		HDD	This LED indicates to indicate internal hard drive activity
		Logging	This indicates activity in the data collection microcontroller. When powered up before logging this is illuminated. When gathering and transmitting data it flashes.
		Alarm Socket	This is a circular 4 pin Bulgin socket which are connected to volt free contacts. The connections are L=normally closed, N=normally open, E=common
		Digital Inputs	These accept a logic signal of 0 or 5v and can be used to attach switches or extra indicators. This needs to be programmed into the system at Scotia.
		Prog	This allows access to the firmware in the unit. This is for Scotia use only.



Counters 3

5 pin 180° DIN socket

For connection to a high speed counter (eg inductive sensor type)

Counters 1&2

7 pin DIN socket

For connection to counters

This input allows either high speed counters (eg inductive sensor type) or slow speed counters (microswitch). The slow speed counter input is debounced to allow accurate counting.

Temperature

5 pin 240 degree DIN socket

For connection to RTDs (Pt100) to provide temperature measurement

4-20 mA Inputs

8 x 8 pin DIN sockets

The ports can take 4-20mA input from any source whether active or passive loop provided the connected plug is wired accordingly.

The plug which attaches to here can be fitted with a serial number chip which uniquely identifies it to the SDAS.

Data received here will be graphed by the SDAS and saved as a data packet to disk.

The SDAS will detect if chipped transmitters are plugged in to the sockets. Those with no chips will be set to off unless they are switched on at the start of data acquire. Transmitters not chipped must be selected before they can be used for acquiring.

SDAS5 Specification

Power supply

Input voltage 90 to 264V 47-63 Hz
Input current 2.1 A @ 110VAC, 1.1A @ 230 VAC
Tx output voltage 24V DC fused at 500mA

Inputs

Counters 2 x High speed counter pulsed input
Slow speed counter with debounced inputs using change over switch

Temperature Pt100 sensor – 4 wire configuration. Identified by electronic serial number.
Uncertainty = 0.2 degrees C

4-20 mA inputs Active or passive loop depending on plug configuration
Identified by electronic serial number
Loop resistor = 100 ohms
Uncertainty = 0.0085% of reading ± 2 lsd.

Digital 0v = Low 5v = High

Operating range -10 to +40 °C

Weight 6.0 kg for 19" rack mounted version
11.2kg for case mounted version


Dimensions Width 320 mm
Height 180 mm
Length 430 mm

All connections must be made prior to switch on. Connect keyboard mouse and monitor and the inputs from the sensors. The SDAS determines what is attached to it at start up and applies this to the data it collects.

If sensors are changed the system MUST be restarted. Hot swapping of inputs is not recommended.

If sensors are changed then a new log must be started.

Scotiadatabox Unit

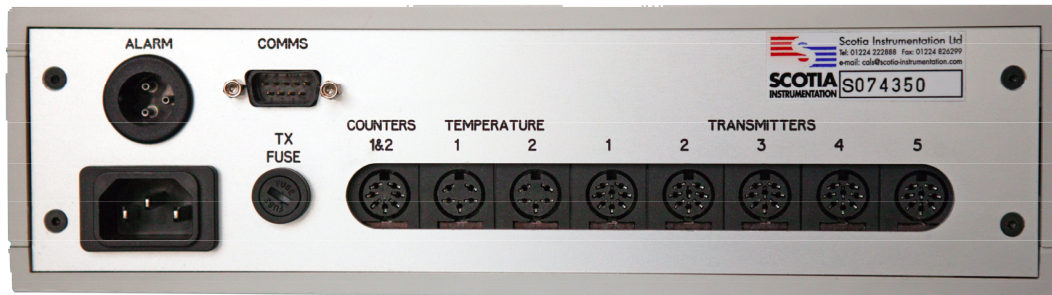

The sockets and specification of the Scotiadatabox are the same as the SDAS except that the Comms port is used for connection to a PC computer. This PC must have an SDAS program installed and running either on from its hard drive or on a plugged in USB stick.

Spares and Accessories List

Stock No Description Addit Description

1018113	Transmitter <10000psi	4-20mA, DIN 43650 plug & socket c/w chip + cable
1021722	Transmitter >10000psi	4-20mA, DIN 43650 plug & socket, c/w chip + cable.
	F250C autoclave fitting,	
1022874	Connector - Free socket connector for alarm option	
1022870	Fuse 125mA , 20mm Anti-surge fuse	
1020405	Leads	1m Extension Lead Pressure
1019859	Leads	10m Extension Lead Pressure
1018392	Leads	10m Extension Lead Temperature Probe
1018391	Leads	15m Extension Lead Temperature
1018390	Leads	15m Extension Lead Pressure
1020954	Leads	20m Extension Lead Pressure
1020955	Leads	20m Extension Lead Temperature
1022872	Leads	3m Network Lead
1022892	Leads	Stroke counter connection lead
1021633		Keyboard & Integral Keypad
1021634		Mains Lead 2 Way, 4m
1021637		USB Printer, Lead & PSU
1022858		17" TFT Monitor
1022877		Temperature probe c/w 1m cable
1022878		Temperature patch c/w 1m cable
1022894		USB stick
1017998	Case	Storage Case for SDAS
1018572	Case	Transit Case for ScotiaDatabox
1022884	Case	Transit Case for SDAS c/w wheels and handle

Appendix 1

Starting the SDAS unit

The SDAS unit is started by switching on the power button. The SDAS has a basic interface along the bottom is a task bar from which you can do various tasks. These include shutting down the SDAS safely, starting the main SDAS application, viewing the SDAS manual, file and printer operations, advanced configuration, noting the operating system version and the current time. The following screen appears when the system starts up.



When you first start the SDAS the above panel will appear. The Control bar along the bottom will stay in place until you launch a program or hover your mouse on it. After that the bar will hide out of sight until you move your mouse close to the bottom of the screen, when it will reappear after a slight delay.

Shutdown - Shutting down the SDAS unit

In order to shut down a soft start SDAS we must first shut down the SDAS program then shutdown the SDAS operating system.


The power button will only turn on the SDAS and will not it turn off.

Do not manually turn off the mains plug or disconnect it.

Shutting down the SDAS operating system will automatically turn off the SDAS unit.

To Shut the SDAS down do the following steps.

Step 1: In the SDAS program return to the main menu screen. Then choose File and Quit. **Do not use** the red x in the top corner of the SDAS program.

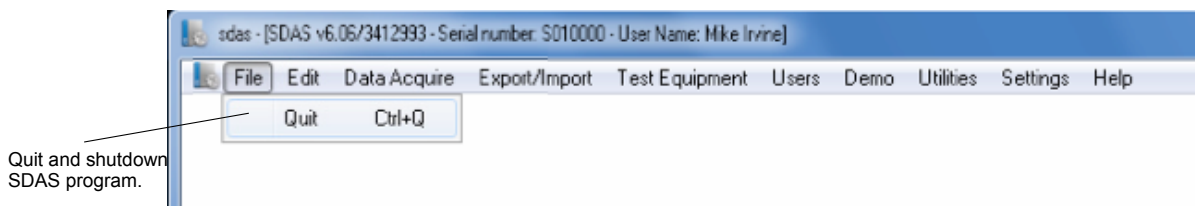


Step 2: Move your mouse to the bottom of the screen and wait for the SDAS bar to appear then press the red and white exit icon.




Step 3: You will be asked to confirm you wish to log off and shutdown. If you see a message saying Please close the 4D application make sure you have closed the SDAS program if you have minimized it click the SDAS button on the bottom bar to bring it back to full screen.

Correct Shutdown

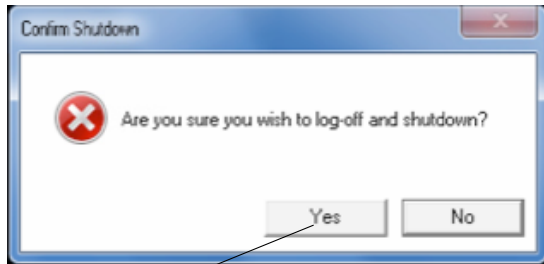


Click yes to shutdown and power off the SDAS

Incorrect Shutdown

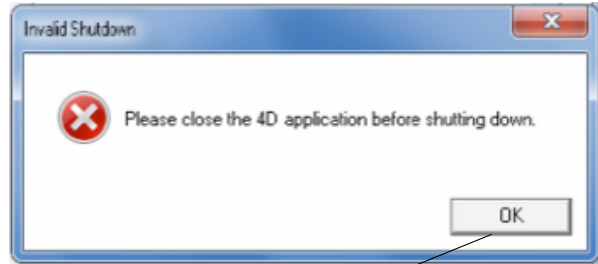


Click ok then go back to step 1 and close the SDAS program.

Step 3: The SDAS will shutdown and you will see a shutdown screen then a black screen for a few seconds then the SDAS should now be powered off correctly. Do not remove power from the SDAS for at least 20 seconds after the black screen has appeared.

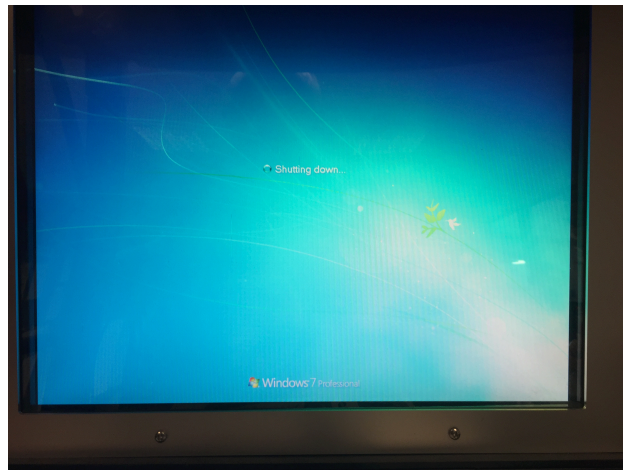


SDAS - Launching the SDAS program

The SDAS button will launch the SDAS application. If the running SDAS application has been minimised for some reason then this button will restore the SDAS application to full size. The SDAS program should never be minimised while logging.

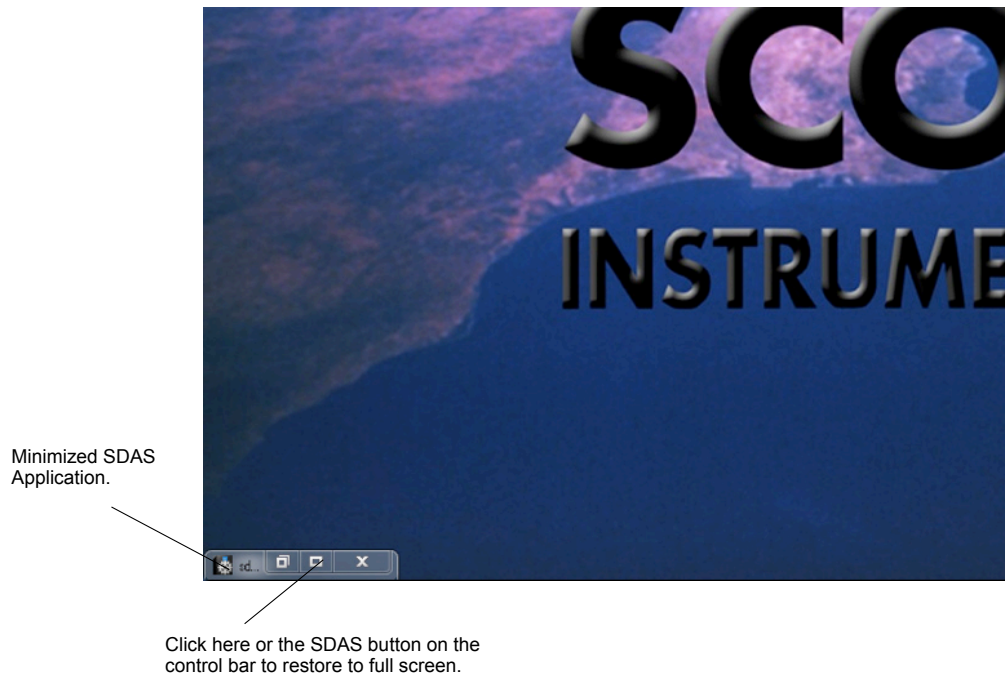

Help - Operation manual pdf

The Help button will launch the SDAS software manual in a new window. When opened or if you move the mouse to the bottom of the help window a tool bar will appear. The help button will also return the help window to fullscreen if you minimize it.

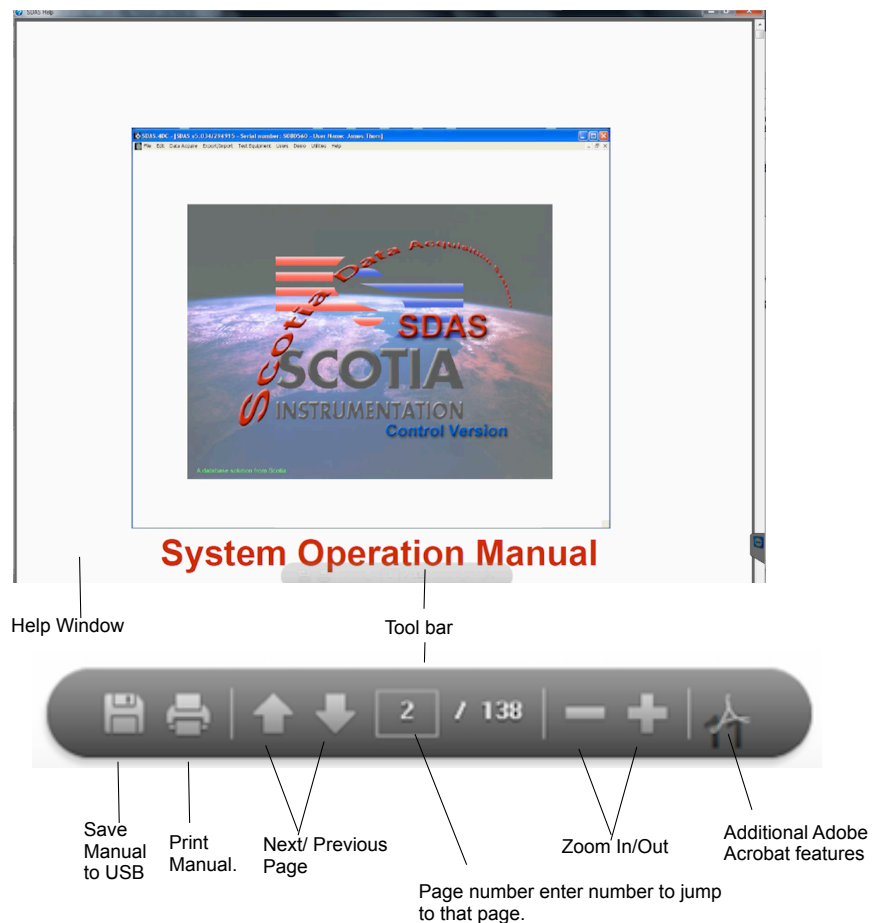

Printers - Changing Printers and clearing the print queue

The Printers button will open the Printers panel. Here you can clear all print jobs and set the default printer. If logged in under the Technician you can also add additional printers.

Default Printer.

Double click any printer icon to set it as the default printer. Note the Default Printer has a Green tick on its icon

Example where three printers are installed Please note the printer name will be different depending on what printer or printers are installed on your SDAS.

Clear all prints in the Queue of the selected Printer.

Add a printer disabled for normal users. Available under technician.

Files - Access local files

The File button will open the file browser will open in a separate window. The file browser is similar to the normal windows file browser with a few exceptions.

The browser will only display Folders, Txt and JPG files. Other files types or those without extensions will be hidden. For this reason please ensure you leave the .txt extensions on any files exported from the SDAS Application or will not be able to access or delete them.

On the local machine only the SDAS folder can be written into. We recommend you use the Export and Import folders for files you wish to store on your SDAS. Please do not adjust the 4D client or 4D software folder as this may break the SDAS application. All folders on a USB device or network share are accessible but the type of files displayed are restricted to TXT, JPG and folders.

Connect and disconnect network Drives. Note this is disabled for normal users but enabled for the technician user.

Import and Export folder. Please put any files to be imported or exported here as some SDAS software screens look here automatically.

The SDAS folder on the local hard drive


USB Drives and Network Drives that have been mapped will appear here.

Name	Size	Type	Date Modified
4D Client		File Folder	4/29/2015 12:46 PM
4D Software		File Folder	2/17/2016 1:50 PM
Export		File Folder	2/26/2014 1:24 PM
Import		File Folder	4/30/2015 9:23 AM

Switch User - Change user


The Switch user button will open the switch user panel. From here you can login as Technician to get access to configuration panels. Pick Technician from the menu and enter the Default password T then click OK. The Default password may have been changed on request so you may have to contact your IT support or whoever is in charge of the SDAS configuration.

Please note the Engineer login is used by Scotia support staff only.

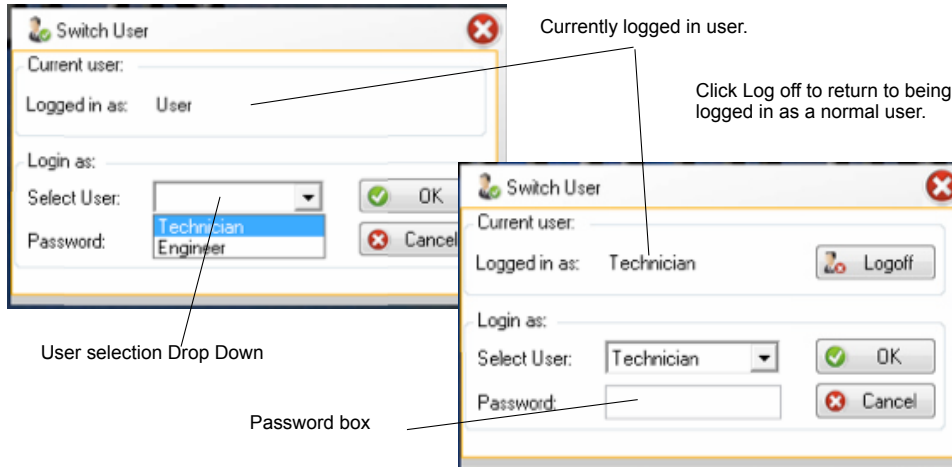

Technician Menus

Logging in as the Technical will cause Panels in the Printers and Files to unlock along with 3 new buttons to appear. The new buttons on the control bar are Settings, Network and Support.

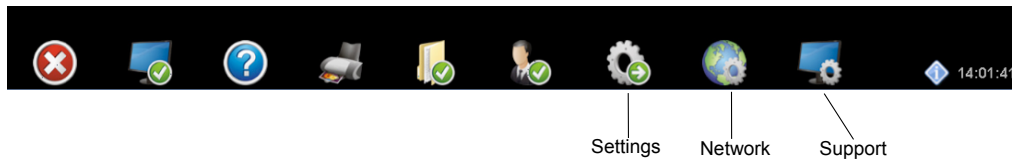


The Settings and network buttons offer a number of configuration options. They should only be accessed by approved staff as adjustments may cause undesirable operation. Make sure to log off when you are finished or you may leave panels open to use by unapproved users.

Technician Printers button

Logging in as the Technical will cause add printer button in the printers panel to unlock. Clicking this will run the windows add printer wizard and you can install USB or network printers to the SDAS unit.

Please note that installation of printers is at your own risk as some 3rd party drivers may result in an unstable or inoperable SDAS.

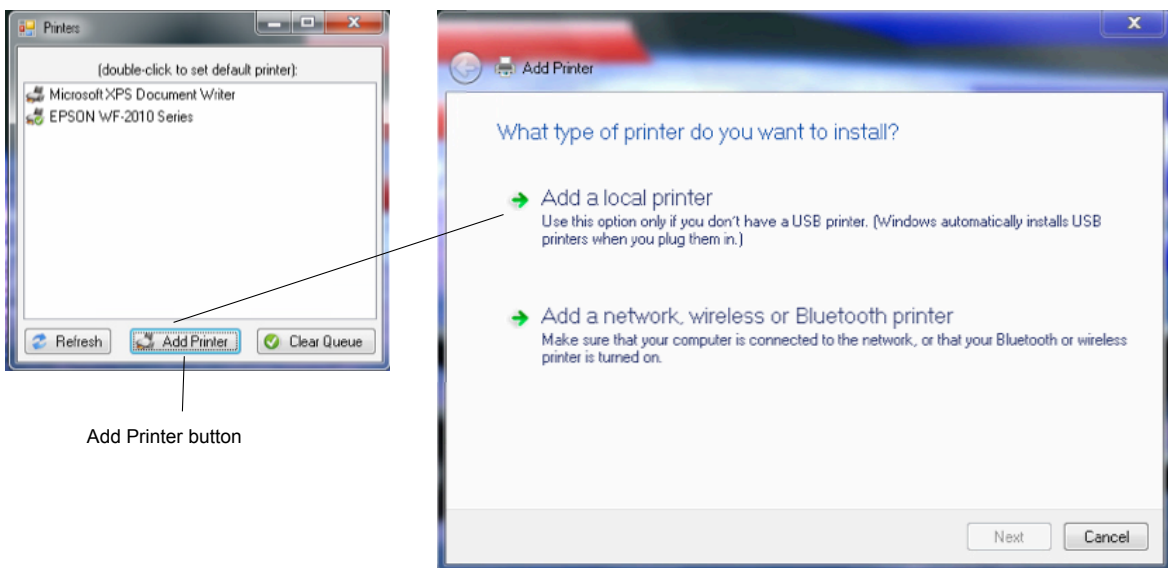

Although almost any printer will work with the SDAS unit some printers cannot be installed by this wizard and will require installation by Scotia Instrumentation technicians.

To be compatible with the SDAS the drivers need to conform to the following requirements.

Drivers must be Windows 7 Pro SP1 compatible.

Drivers must be INF file format.

Drivers must not install non standard application to work such as system tray based ink monitors or replacement printing systems, the operating system is heavily customized and these kind of applications may result in a non bootable system.

Most basic Hewlett Packard INF Driver only packages are suitable. The SDAS also has some printer drivers bundled with it. However there are a few caveats.

Generic printer drivers that require configuration after installation can be installed but there will be no way configure the driver after installation these include the HP universal network printer driver.

EXE Installers cannot be used unless installed by Scotia Technicians in engineer mode.


The wizard may prompt for files not present in the OS install and these will need to be extracted from a Windows 7 32bit Pro SP1 DVD or may be present in the C:\windows\system32\drvstore folder.

Technician Files button

Logging in as Technician also unlocks the Map Network Drive and Disconnect network Drive buttons in the Files Panel.

Mapping a network drive will make an SMB share accessible to all users of the SDAS.

Click Map Network Drive in the top right of the File explorer and the Map Network Drive window will appear.

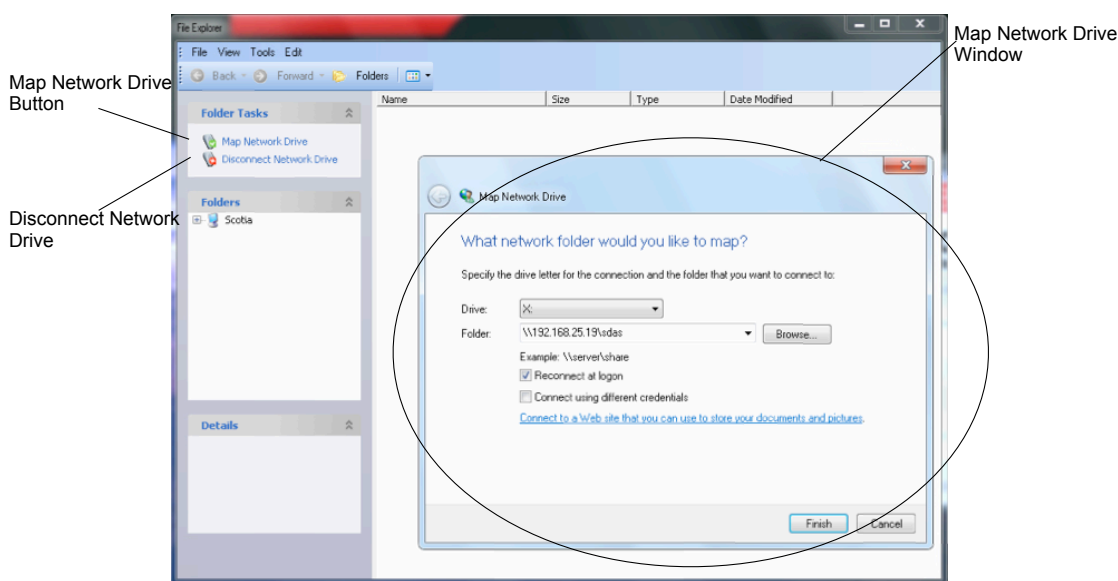

Simply choose the drive letter you want to assign to the network share E: through to Z: a possible 22 connections.


Although you can select D: as a 23rd connection it is recommended that you do not use this but leave it for use with USB devices.

After you have selected the drive letter you wish to use enter the UNC path of the folder you wish to connect to. For example \\server.scotia.local\sdas or \\192.168.0.1\share.


You can also use the "Browse..." button to find the SMB network share you wish to use but this may have difficulty finding your share depending on how your local network is setup and network security policies. Consult your IT department for UNC paths.

Check the Reconnect at logon if you wish the SDAS to remember the connection if you do not check this option the SDAS will forget the connection when it is restarted.


After choosing your Drive letter and entering the path and checking Reconnect at logon press the "Finish" button. You will then receive a prompt for the user name and password for the share you are trying to access. In some cases the user name will need a qualification to work for example "scotia.local\sdasuser", "192.168.0.1\sdasuser" or "[sdasuser@scotia.local](#)". Please consult your IT department for the correct username and password.

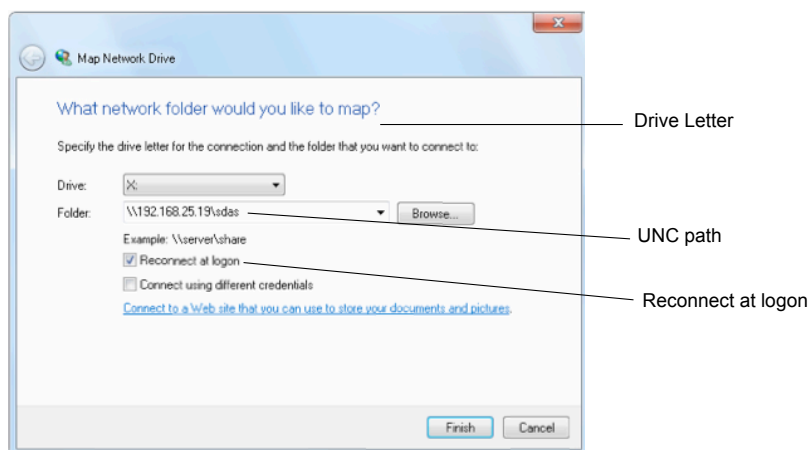

After mapping a drive you may need to close the File browser and reopen it for the share to appear. If your network share still does not appear please ensure you checked reconnect at logon then restart the SDAS. The network share will appear in the file browser as NW Drive and the letter you chose. Multiple network shares you have mapped will appear in alphabetical order.

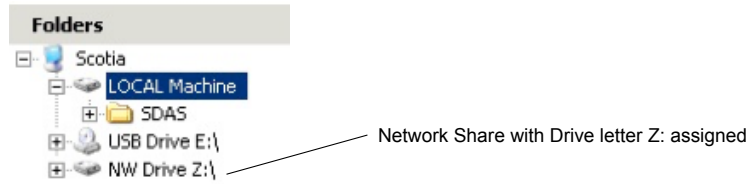


Clicking Disconnect Network Drive will open a prompt windows asking you to select the drive you wish to disconnect. Simply select the drive you wish to remove then click ok. You may need to restart the File browser or SDAS for this to take effect.

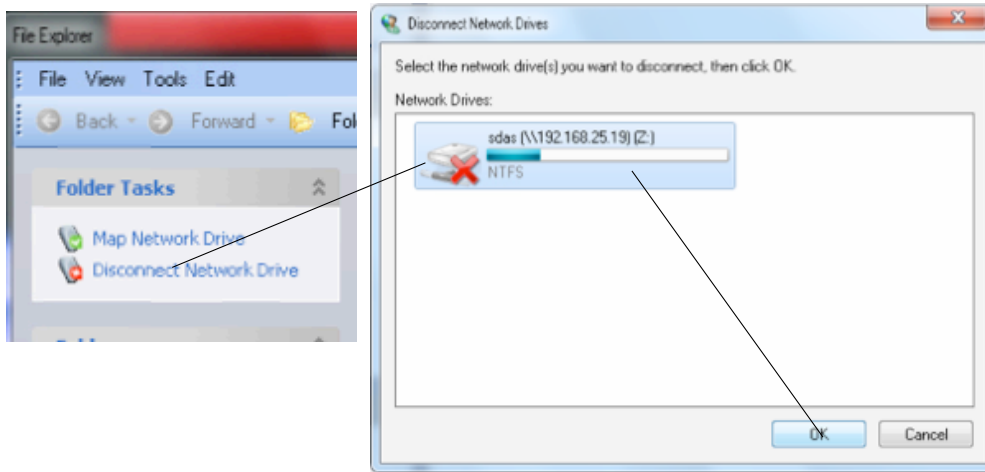


Technician Settings button

The settings button will give you access to two Tabs SDAS and Date/Time.

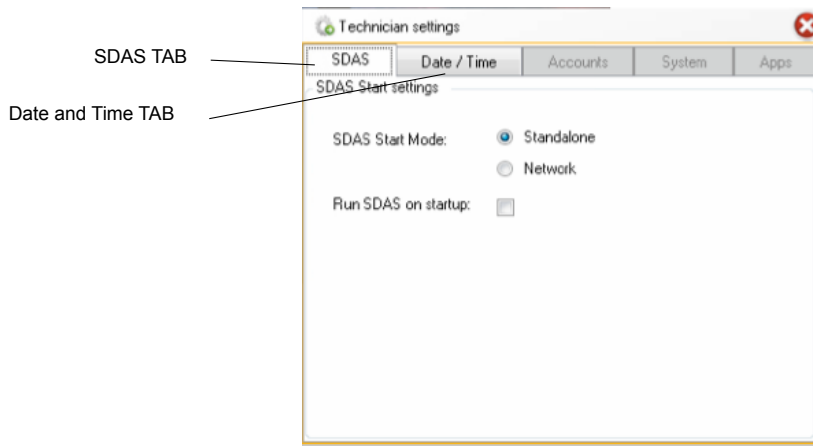

The SDAS tab lets you customize the SDAS startup to run in either local stand alone mode or Network mode. **Please note Network mode is not currently available in version 6.** You can also set the SDAS program to Immediately start when the SDAS is turned on. Note this will also immediately stop the ability to edit the time and date.

The Date/Time tab will allow you to change the time and date on the SDAS. This button will only work for 12 minutes after the SDAS is turned on or until the SDAS program is launched. The button will disable and grey out as shown below after 12 minutes or the SDAS program launch. You will need to restart the SDAS unit to reactivate it. Please note that if in the SDAS tab "Run SDAS on startup" is enabled the adjust time button will be permanently disabled until it is turned off and the unit restarted.

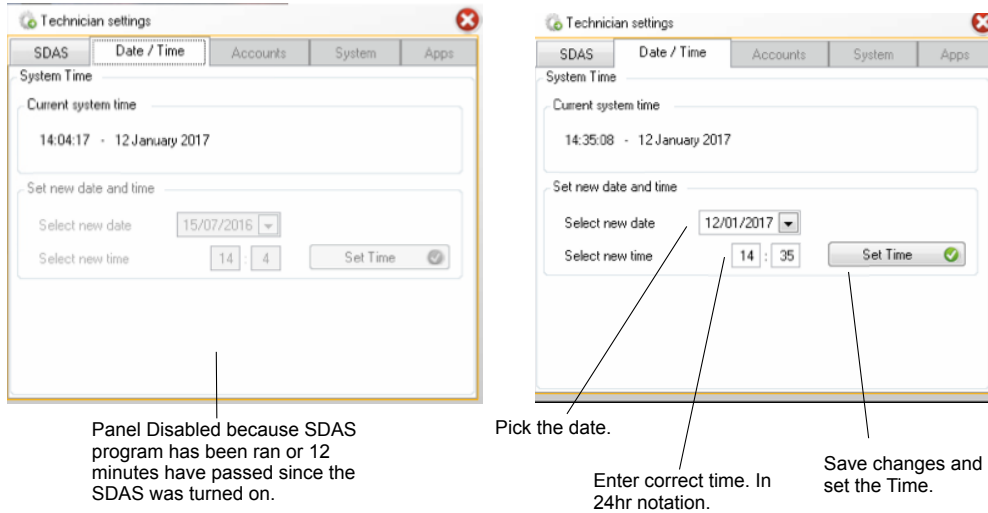


Please note the Time panel does not support automatic changes such as BST.

You should manually correct the time if this is required. This is to stop data being lost if logging when the clocks go back or forward.

Technician Network button


Clicking the Network button will open the TCP/IP configuration panel in a new window.

By default SDAS units are set to use DHCP and if your network is configured to support DHCP you not need to do any further configuration.

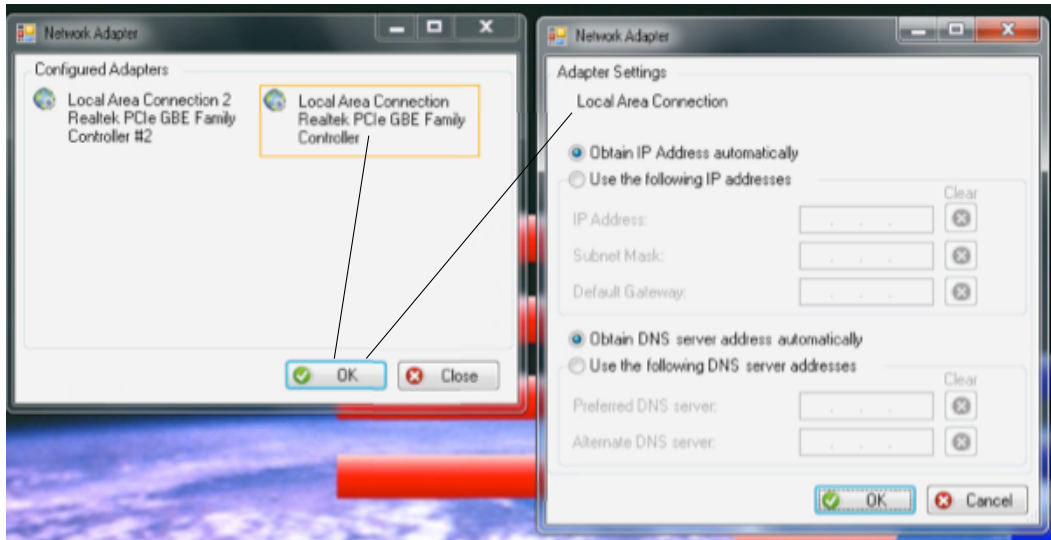

If you require you can set the SDAS unit to have a Static IP address. To do this simply check the "Use the following IP Address" radio button and enter the IP address, Subnet Mask and Default Gateway you wish to use then click "Use the following DNS server addresses" and enter the IP addresses of your primary and secondary DNS servers.

Technician Support button

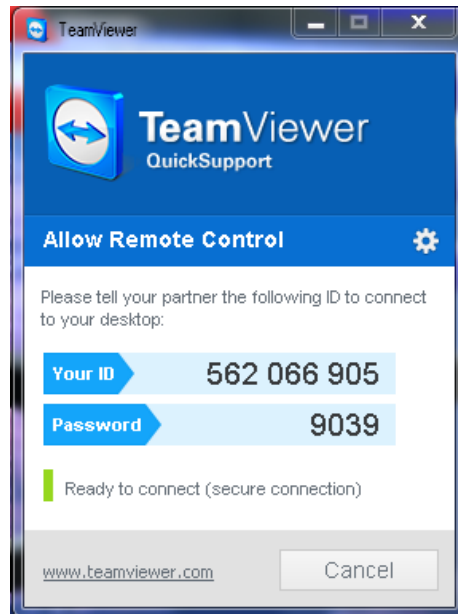

Clicking support button launches the Scotia Remote Support application in a new window.

The Scotia Remote Support application allows a Scotia Technician to take control of your SDAS remotely over the internet.

The remote support application includes full encryption, based on RSA private-/public key exchange and AES (256 Bit) session encoding. This technology is based on the same standards as https/SSL and is considered completely safe by today's standards.

The key exchange also guarantees a full client-to-client data protection.

In addition to the PartnerID the support application generates a session password that changes with every software start to provide additional security against unauthorized access to a remote system. Security relevant functions like file transfer require additional, manual confirmation of the remote partner. Also it is not possible to invisibly control the SDAS. For data protection reasons the person operating the SDAS has to be able to detect when someone is accessing the machine.

All support sessions have to be initiated from the SDAS.

A fully working internet connection is required for the support application to work for this reason the SDAS must be set to use DHCP or have correct Static IP and DNS settings. The support application is general able to traverse Firewalls and NAT without further configuration. However some IT departments purposely block Teamviewer. Proxy server use may require additional configuration.

To initiate a Support session you will need to launch the Support application and provide the ID and Password to a Scotia engineer, these are clearly displayed in the SDAS Remote Support window. Please note that if you do not have a maintenance agreement you may be charged for remote support.

Appendix 2

4D Error messages

When the system hits a bug or develops an error of some kind then system error messages appear which look like the screen below. There are buttons on the screen which give options. If you choose to Continue then you should do so only to allow you to complete an immediate task.

YOU SHOULD NOT CONTINUE TO DO ANY IMPORTANT LOGGING WORK

These events are very unusual and often occur as a result of a combination of tasks which may not have been covered in testing. Please capture the error message. Please make sure to expand the little plus symbol next to the Details text as this often provides more information.

A good method of doing that is to simply use a camera or the camera on a phone. Do a close picture of the message and a longer shot of the whole screen. It would be very helpful if you could note what task you were doing and any unusual thing that happened.

Report the error to Scotia immediately either by phone or email. Do not continue to use the SDAS system until either the problem is fixed with an upgrade or you are advised by Scotia that you can continue.

The error showing below was as a result of a program bug

